



(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention  
of the grant of the patent:  
**16.11.2005 Bulletin 2005/46**

(21) Application number: **00960950.4**

(22) Date of filing: **13.09.2000**

(51) Int Cl.7: **A61N 1/36**

(86) International application number:  
**PCT/IL2000/000566**

(87) International publication number:  
**WO 2001/066183 (13.09.2001 Gazette 2001/37)**

(54) **BLOOD GLUCOSE LEVEL CONTROL**  
**STEUERUNG DES BLUTZUCKERSPIEGELS**  
**REGULATION DU TAUX DE GLUCOSE DANS LE SANG**

(84) Designated Contracting States:  
**DE FR GB IT**

(30) Priority: **05.03.2000 WOPCT/IL00/00132**

(43) Date of publication of application:  
**11.12.2002 Bulletin 2002/50**

(73) Proprietor: **IMPULSE DYNAMICS N.V.**  
**Curacao (AN)**

(72) Inventors:  
• **DARVISH, Nissim**  
**30850 Hof-Hacarmel (IL)**  
• **HAREL, Tami**  
**34862 Haifa (IL)**  
• **FELSEN, Bella**  
**34355 Haifa (IL)**  
• **GLASBERG, Offer**  
**32447 Haifa (IL)**

(74) Representative: **van Westenbrugge, Andries et al**  
**Nederlandsch Octrooibureau**  
**P.O. Box 29720**  
**2502 LS The Hague (NL)**

(56) References cited:

**WO-A-93/02743** **WO-A-98/57701**  
**WO-A-99/03533** **US-A- 5 995 872**

- **HOLST JENS J ET AL: "Nervous control of pancreatic endocrine secretion in pigs" ACTA PHYSIOLOGICA SCANDINAVICA, vol. 111, January 1981 (1981-01), pages 1-7, XP000980527 Oxford, UK**
- **HOLST JENS J ET AL.: "Nervous control of pancreatic endocrine secretion in pigs" ACTA PHYSIOLOGICA SCANDINAVICA, vol. 111, January 1981 (1981-01), pages 9-14, XP000980528 Oxford, UK**
- **PARK HS, LEE YL, KWON HY, CHEY WY, PARK HJ: "Significant cholinergic role in secretin-stimulated exocrine secretion in isolated rat pancreas" AMERICAN JOURNAL OF PHYSIOLOGY, vol. 274, no. 2 Pt 1, February 1998 (1998-02), pages G413-G418, XP002157834**
- **SINGH J ET AL.: "Effects of islet hormones on nerve-mediated and acetylcholine-evoked secretory responses in the isolated pancreas of normal and diabetic rats" INTERNATIONAL JOURNAL OF MOLECULAR MEDICINE, vol. 1, no. 3, March 1998 (1998-03), pages 627-634, XP000980499**

Note: Within nine months from the publication of the mention of the grant of the European patent, any person may give notice to the European Patent Office of opposition to the European patent granted. Notice of opposition shall be filed in a written reasoned statement. It shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

## Description

### RELATED APPLICATIONS

[0001] This application claims the benefit under 119 (e) of US provisional application 60/123,532, filed March 5, 1999. This application is a continuation-in-part of PCT application PCT/IL00/00132, filed on March 5, 2000, which designates the US. This application is also related to WO 99/03533.

### FIELD OF THE INVENTION

[0002] The present invention is related to the field of controlling blood serum glucose levels, especially by application of electric fields to a pancreas, to control insulin output.

### BACKGROUND OF THE INVENTION

[0003] Control of insulin secretion is very important, as there are many living diabetes patients whose pancreas is not operating correctly. In some type of diabetes, the total level of insulin is reduced below that required to maintain normal blood glucose levels. In others, the required insulin is generated, but only at an unacceptable delay after the increase in blood glucose levels. In others, the body is, for some reason, resistant to the effects of insulin.

[0004] Although continuous control (e.g., avoiding dangerous spikes and dips) of blood glucose level is desirable, it cannot currently be achieved in some patients.

[0005] The insulin secretion process operates as follows: glucose levels in the blood are coupled to depolarization rates of beta islet cells in the pancreas. It is postulated that when there is a higher glucose level, a higher ratio of ATP/ADP is available in the beta cell and this closes potassium channels, causing a depolarization of the beta cell. When a beta cell depolarizes, the level of calcium in the cell goes up and this elevated calcium level causes the conversion of pro-insulin to insulin and causes secretion of insulin from the cell.

[0006] The beta cells are arranged in islets, within a reasonable range of blood glucose levels, an action potential is propagated in the islet. Generally, the electrical activity of a beta cell in an islet is in the form of bursts, each burst comprises a large number of small action potentials.

[0007] In PCT publication WO 99/03533, it was suggested to reduce the output of a pancreas using a non-excitatory electric field.

[0008] PCT publication WO 98/57701 to Medtronic, suggests providing a stimulating electric pulse to an islet, causing an early initiation of a burst and thus, increasing the frequency of the bursts and increasing insulin secretion.

[0009] The above PCT publication to Medtronic suggests providing a stimulating (e.g., above stimulation

threshold) pulse during a burst, thereby stopping the burst and reducing insulin secretion. This publication also suggests stimulating different parts of the pancreas in sequence, thereby allowing unstimulated parts to rest.

[0010] However, one limitation of the methods described in the Medtronic PCT publication is that increasing the burst frequency increases the level of intracellular calcium in the beta cells over a long period of time, without the level being allowed to go down, during intraburst intervals. This increase may cause various cell death mechanisms to be activated and/or otherwise upset the normal balance of the beta cell, eventually killing the cell. In addition, such high calcium levels may cause hyper-polarization of beta cells, thereby reducing insulin secretion and preventing propagation of action potentials. To date, no working electrical pancreatic control device is known.

[0011] Diabetologia (1992) 35:1035-1041, for example, describe the interaction of the various hormones generated by the pancreas. Insulin enhances glucose utilization, thereby reducing blood glucose levels. Insulin also stimulates the secretion of glucagon which causes the liver to secrete glucose, increasing the blood glucose level. Somatostatin reduces the secretion of both insulin and glucagon. This publication also describes an experiment in which sympathetic nervous stimulation caused an increase in Somatostatin secretion. It is suggested in this paper that normal glucose levels in a healthy human may be maintained with the aid of glucagon secretion.

### SUMMARY OF THE INVENTION

[0012] An aspect of some embodiments of the invention relates to selective and/or integrative control of the various hormones generated by the pancreas and which affect blood glucose level, to provide a control of blood glucose levels. The control may be achieved using pure electrical stimulation, or possibly using one or more pharmaceuticals and/or other molecules to interact with the electrical stimulation in a desired manner. The pharmaceuticals may prevent the pancreatic cells from producing and/or secreting a hormone. Alternatively, the pharmaceuticals may prevent the action of the hormone, for example by blocking the receptors or disabling the hormone. Alternatively or additionally, hormones, such as insulin, Somatostatin or glucagon may be provided from outside the body or using an insulin pump. In some embodiments of the invention, the control is non-excitatory (defined below). In other embodiments of the invention, the control is excitatory or a combination of excitatory and non-excitatory control.

[0013] In some exemplary embodiments of the invention, the control is not merely of the blood glucose levels but also of the hormone levels required to provide a satisfactory physiological effect, rather than merely prevention of symptomatic effects of incorrect blood glucose

levels. Such control may be effected, for example to achieve desirable short term effects alternatively or additionally to achieving desirable long term effects. This type of positive control of two parameters should be distinguished from merely controlling blood glucose by varying the insulin level. Such mere controlling may not allow both desired blood glucose levels and insulin levels to be achieved, possibly leading to over-exertion of the pancreas.

**[0014]** It is hypothesized that one possible reason for lack of success of nervous or direct stimulation of the pancreas for glucose control is the simultaneous and non-selective effect of the stimulation on the secretion of several different hormones, reducing the effectiveness of the hormones secreted and/or overworking the pancreas.

**[0015]** In an exemplary embodiment of the invention, the secretion of a counteracting type of hormone (e.g., glucagon or insulin) is suppressed, to prevent feedback interactions whereby the secretion of a target hormone (e.g., insulin or glucagon) increases the secretion of the counteracting hormone.

**[0016]** Alternatively or additionally, the stimulation of secretion of the target hormone is maintained at low enough levels that do not cause a significant secretion of the counteracting hormone. The secretion time may be extended, so that the total amount of hormone is sufficient for a desired result.

**[0017]** Alternatively or additionally, the stimulation of secretion of the target of hormone is controlled to be in bursts that are not long enough to stimulate a significant secretion of the counteracting hormone. Alternatively, the secretion may be made sustained, to purposely cause secretion and/or production of the counteracting hormone to a desired degree.

**[0018]** Alternatively or additionally, the secretion of the target hormone is maintained at a high enough level to overcome the counteracting effects.

**[0019]** Alternatively or additionally, the stimulation of secretion of the target hormone is maintained at a high enough level to cause the generation of significant amounts of a secretion limiting hormone (e.g., Somatostatin), which secretion prevents the secretion of the counteracting hormone, but is not sufficient to prevent the stimulation from releasing of the target hormone.

**[0020]** Alternatively or additionally, the secretion of several of pancreatic hormones is suppressed by hyper-polarizing the pancreas. Such hyper-polarization can be electrical in nature or chemical. For example, Diazoxide causes hyper-polarization and reduces activity in the pancreas.

**[0021]** Alternatively or additionally, beta cell response (e.g., insulin secretion) to high blood glucose levels is dampened, rather than blocked, so as to prevent hypoglycemia. Alternatively or additionally, glucagon secretion is provided to prevent hyperglycemia, when high insulin levels persist in spite of reduced glucose intake. In some cases, damping of Insulin response and/or pro-

vision of glucagon are used to prevent overshoots caused, for example, by a delayed response to the artificial control of the pancreas. In some cases, the insulin (or other hormone) increasing or decreasing pulse is applied and/or removed gradually (e.g., with regard to effect or temporal frequency), to prevent such an overshoot. Alternatively or additionally, an active measure, such as providing an antagonistic hormone, is used.

**[0022]** An aspect of some embodiments of the invention relates to effecting control of Insulin and/or glucose blood levels by controlling glucagon secretion. In an exemplary embodiment of the invention, such increased glucagon secretion is used to increase blood glucose levels, instead of insulin secretion reduction or additional to it. Optionally, the secretion of glucagon is limited so as not to cause a complete depletion of glucose sources in the liver. Alternatively or additionally, Insulin secretion is stimulated by an increase in glucagon secretion. In an exemplary embodiment of the invention, both a desired glucose level and a desired insulin level can be achieved simultaneously, by suitably controlling glucagon secretion. Alternatively or additionally, the need for abnormally high levels of insulin are prevented by not stimulating glucagon secretion. In some cases, insulin secretion is provided to prompt the creating of glucose stores in the liver or glucagon is provided to deplete such stores.

**[0023]** In some exemplary embodiments of the invention, controlling both glucose levels and insulin levels allows control over effects of Insulin other than blood glucose level, for example effects on lipid metabolism, gluconeogenesis in liver, ketogenesis, fat storage, glycogen formation.

**[0024]** Alternatively or additionally, the liver may be overwhelmed with glucose and/or insulin, without associated hyperglycemia, so as to force complete filling of glycogen reserves and/or prevent hepatic absorption of glucose at a later time.

**[0025]** Alternatively or additionally, insulin levels may be reduced so that less glycogen is stored in the liver. This may be useful in von Gierke's over-storage disorder and/or in other over-storage disorders.

**[0026]** An aspect of some embodiments of the invention relates to mapping the response and/or feedback behavior of a pancreas. Such mapping may be for, for example a particular patient, and/or for a type of patient and/or pancreatic disorder.

**[0027]** In an exemplary embodiment of the invention, one or more of the following properties of a pancreas is determined:

- (a) the interaction between two or more hormones, including one or more of the amplification gain (positive or negative), the effect of short vs. long sustained changes in one hormone level on another, delay times for effect of one hormone on another, and/or natural sequences of hormone activation;
- (b) response of hormone secretion and/or produc-

tion to various stimulatory and inhibitory effects, such as electrical fields, pharmaceuticals and/or nervous stimulation;

(c) the effect of glucose levels, previous stimulation of the pancreas and/or pharmaceutical levels on the hormone interactions and responses to stimulation and to levels of other pancreatic hormones and/or other physiological parameters, for example levels of digestive enzymes;

(d) burst ability vs. hormone creating ability, including, for example, intra-cellular hormone and pre-hormone storage capacity and/or time constants;

(e) different behavior of different parts of the pancreas; and

(f) electrical activity of all or some of the pancreas.

**[0028]** In some embodiments, the mapping also determines the effect of non-pancreatic hormones, for example pituitary, thyroid and adrenal hormones. Some of these hormones may increase or reduce blood glucose level by direct effect on the liver.

**[0029]** In an exemplary embodiment of the invention, a direct measurement of absolute or relative hormone levels and/or a measurement of glucose levels and/or other physiological parameters, is used to determine the effect of various stimulation. Such measurements may be on-line or off-line. In an exemplary embodiment of the invention, a fiber-optic chemical sensor is used to assay hormone levels. Alternatively or additionally, an anti-body based test is used. In an exemplary embodiment of the invention, the controller includes a port or a guide wire to the pancreatic and/or portal circulatory system. Possibly, the port or guide wire exits the body, reach until just under the skin and/or open into a body lumen, for easy access. Such a port or guide wire may be adapted for guiding a catheter, for removing hormone laden blood from the pancreas. The catheter and/or guide wire may be removed once a mapping stage is over. Alternatively or additionally, the port is used to guide an endoscope, for implantation and/or repositioning of sensors and/or electrodes.

**[0030]** Alternatively or additionally to measuring intra-pancreatic interactions, the adaptation of the pancreas to various physiological states and/or the adaptation of the body to various pancreatic states and/or blood hormone levels, is also measured. Such measuring may be performed in a laboratory. Alternatively or additionally, an ambulatory or implanted device is provided to a patient, to measure the above pancreatic behaviors over time.

**[0031]** In an exemplary embodiment of the invention, the above measured behaviors are used as parameters for a predictive model of the behavior of the pancreas. Alternatively or additionally, a new model, for example a neural network type model is created from the measurements. Such a model is possibly used to predict the effect of a therapy and/or to choose between alternative therapies. In an exemplary embodiment of the invention,

such a model is used to select a therapy for glucose level reduction which increases insulin secretion but does not increase glucagon secretion.

**[0032]** An aspect of some exemplary embodiments relates to controlling pancreatic behavior indirectly by controlling the flow of blood to the pancreas, for affecting hormone generation and secretion and/or by controlling blood flow from the pancreas, to effect hormone dissemination and/or local levels of hormone in the pancreas. In an exemplary embodiment of the invention, the blood flow is controlled using non-excitatory electrical fields that selectively contract or relax arteries and/or veins to, from or inside some or all of the pancreas.

**[0033]** An aspect of one exemplary embodiment of the invention relates to a method of increasing insulin secretion, while avoiding unacceptable calcium level profiles. In an exemplary embodiment of the invention, insulin output is increased by extending a burst duration, while maintaining a suitably lengthy interval between bursts, thus allowing calcium levels to decay during the interval. Alternatively or additionally, insulin output is increased by increasing the effectiveness of calcium inflow during a burst, possibly without changing the burst frequency and/or duty cycle. Alternatively, in both methods, the burst frequency may be reduced and/or the interval increased, while allowing higher insulin output levels or maintaining same output levels.

**[0034]** In an exemplary embodiment of the invention, the effects on insulin secretion are provided by applying a non-excitatory pulse to at least part of the pancreas. As used herein the term non-excitatory is used to describe a pulse that does not generate a new action potential, but may modify an existing or future potential. This behavior may be a result of the pulse, amplitude, frequency or pulse envelope, and generally also depends on the timing of the pulse application. It is noted that a single pulse may have excitatory and non-excitatory parts. For example a 100 ms pacing pulse, may cease to have a pacing effect after 20 ms and have real non-excitatory effects after 40 ms.

**[0035]** The pulse may be synchronized to the local electrical activity, for example, to bursts or to individual action potentials. Alternatively or additionally, the pulse may be synchronized to the cycle of changes in insulin level in the blood (typically a 12 minute cycle in healthy humans). Alternatively, the pulse may be unsynchronized to local or global pancreatic electrical activity. Alternatively, the applied pulse may cause synchronization of a plurality of islets in the pancreas, for example by initiating a burst. A two part pulse may be provided, one part to synchronize and one part to provide the non-excitatory activity of the pulse. Although the term "pulse" is used, it is noted that the applied electric field may have a duration longer than an action potential or even longer than a burst.

**[0036]** An aspect of some exemplary embodiments of the invention relates to reducing calcium levels in beta islet cells. In an exemplary embodiment of the invention,

the levels are reduced by providing an oral drug. Alternatively, the levels are reduced by increasing the interval between bursts. The intervals may be increased, for example, by suppressing bursts of action potentials, for example using excitatory or non-excitatory pulses. Alternatively, an electro-physiological drug is provided for that purpose. For example, Procainamide HCL and Quinidine sulfate are Na channel antagonists, Minoxidil and Pinacidil are K channel activators, and Amiloride HCL is an Na channel and epithelial antagonist. Other suitable pharmaceuticals are known in the art, for example as described in the RBI Handbook of Receptor Classification, and available from RBI inc. This reduction in calcium levels may be performed to reduce the responsiveness of the pancreas to glucose levels in the blood. Alternatively or additionally, this reduction is used to offset negative side effects of drugs or other treatment methods and/or to enforce a rest of at least a part of the pancreas. Alternatively or additionally, this reduction may be offset by increasing the effectiveness of insulin secretion.

**[0037]** An aspect of some exemplary embodiments of the invention relates to pacing at least a portion of the pancreas and, at a delay after the pacing, applying a non-excitatory pulse. The non-excitatory pulse may be provided to enhance or suppress insulin secretion or for other reasons. In an exemplary embodiment of the invention, the pacing pulse provides a synchronization so that the non-excitatory pulse reaches a plurality of cells at substantially a same phase of their action potentials. A further pulse, stimulating or non-excitatory may then be provided based on the expected effect of the non-excitatory pulse on the action potential.

**[0038]** An aspect of some exemplary embodiments of the invention relates to simultaneously providing pharmaceuticals and electrical control of a pancreas. In an exemplary embodiment of the invention, the electrical control counteracts negative effects of the pharmaceuticals. Alternatively or additionally, the pharmaceutical counteracts negative effects of the electrical control. Alternatively or additionally, the electrical control and the pharmaceutical complement each other, for example, the pharmaceutical affecting the insulin production mechanisms and the electrical control affecting the insulin secretion mechanism. The electrical control and/or the pharmaceutical control may be used to control various facets of the endocrine pancreatic activity, including one or more of: glucose level sensing, insulin production, insulin secretion, cellular regeneration, healing and training mechanisms and/or action potential propagation. In an exemplary embodiment of the invention, electrical and/or pharmaceutical mechanisms are used to replace or support pancreatic mechanisms that do not work well, for example, to replace feedback mechanisms that turn off insulin production when a desired blood glucose level is achieved. The pharmaceuticals that interact with the pancreatic controller may be provided for affecting the pancreas. Alternatively, they

may be for other parts of the body, for example for the nervous system or the cardiovascular system.

**[0039]** An aspect of some exemplary embodiments of the invention relates to activating pancreatic cells in various activation profiles, for example to achieve training, regeneration, healing and/or optimal utilization. In an exemplary embodiment of the invention, such activating can include one or more of excitatory pulses, non-excitatory pulses and application of pharmaceuticals and/or glucose. It is expected that diseased cells cannot cope with normal loads and will degenerate if such loads are applied. However, by providing sub-normal loads, these cells can continue working and possibly heal after a while using self healing mechanisms. In particular, it is expected that certain diseased cells, when stimulated at at least a minimal activation level, will heal, rather than degenerate. Alternatively or additionally, it is expected that by stressing cells by a certain amount, compensation mechanisms, such as increase in cell size, response speed and profile to glucose levels, cell effectiveness and/or cell numbers, will operate, thereby causing an increase in insulin production capability, insulin response time and/or other desirable pancreatic parameters. The appropriate activation profiles may need to be determined on a patient by patient basis. Possibly, different activation profiles are tested on one part of the pancreas, and if they work as desired, are applied to other parts of the pancreas. Those other parts of the pancreas may be suppressed during the testing, to prevent over stressing thereof. Alternatively, they may be maintained at what is deemed to be a "safe" level of activity, for example by electrical control or by pharmaceutical or insulin control.

**[0040]** An aspect of some exemplary embodiments of the invention relates to electrically affecting and preferably controlling insulin generation, alternatively or additionally to affecting insulin secretion. In an exemplary embodiment of the invention, insulin production is enhanced by "milking" insulin out of beta cells so that their supplies of insulin are always under par. Alternatively or additionally, by under-milking such cells (e.g., prevention of secretion), insulin production is decreased. In some patients opposite effects may occur - over milking will cause a reduction in insulin production and/or under-milking will increase insulin production. Alternatively, insulin production is suppressed by preventing a cell from secreting insulin (e.g., by preventing depolarization), thereby causing large amount of insulin to stay in the cell, and possibly, prevent further production of insulin. Such mechanisms for stopping the production of insulin have been detected in pancreatic cells.

**[0041]** In an exemplary embodiment of the invention, by causing a cell to store a large amount of insulin, a faster response time can be achieved, when large amounts of insulin are required, for example to combat hyperglycemia. The cells can then be systemically depolarized to yield their stores of insulin. Possibly, a plurality of pancreatic cells (the same or different ones at

different times) are periodically set aside to serve as insulin burst providers.

**[0042]** Alternatively or additionally, suppression of insulin output is used during medical procedures, to prevent hypoglycemia. Alternatively or additionally, suppression or enhancement of insulin output is used to overwork pancreatic tumor cells, so they die from over production or from over-storage of insulin. In some cases, the overworking of cells caused by cycling demand may be used as a form of stress to weaken cells, and in combination with another stress source, kill the cells. Alternatively or additionally, suppression of insulin output is used to reduce the activity of an implanted pancreas or pancreatic portion, to assist in its getting over the shock of transplantation.

**[0043]** An aspect of some exemplary embodiments of the invention relates to controlling the propagation of action potentials and/or other parameters of action potentials in islet cells, alternatively or additionally to controlling parameters of burst activity. In an exemplary embodiment of the invention, a pulse, optionally synchronized to individual action potentials in an islet, is used to control the action potential, for example to increase or decrease its plateau duration. Alternatively or additionally, a reduction in action potential frequency towards the end of a burst is counteracted, for example by pacing the cells to have a desired frequency or to be more excitable.

**[0044]** In an exemplary embodiment of the invention, action potential propagation is controlled, for example enhanced or blocked, by selectively sensitizing or desensitizing the beta cells in an islet, using chemical and/or electrical therapy. Enhancement of action potential may be useful for increasing insulin production rates, especially if the glucose sensing mechanism in some cells are damaged. Suppression of action potential propagation is useful for preventing insulin production and/or enforcing rest.

**[0045]** An aspect of some exemplary embodiments of the invention relates to indirectly affecting the pancreatic activity by changing pancreatic response parameters, such as response time to increases in glucose level and response gain to increases in glucose level. Thus, for example, a non-responsive pancreas can be sensitized, so that even small changes in glucose level will cause an outflow of insulin. Alternatively, a weak or over-responsive pancreas can be desensitized, so that it isn't required to generate (large amounts of) insulin for every small fluctuation in blood glucose level. It is noted that the two treatments can be simultaneously applied to different parts of a single pancreas.

**[0046]** An aspect of some exemplary embodiments of the invention relates to synchronizing the activities of different parts of the pancreas. Such synchronization may take the form of all the different parts being activated together. Alternatively, the synchronization comprises activating one part (or allowing it to become active) while suppressing other parts of the pancreas (or allow-

ing them to remain inactive). In an exemplary embodiment of the invention, the synchronization is applied to enforce rest on different parts of the pancreas. Alternatively or additionally, the synchronization is provided to selectively activate fast-responding parts of the pancreas or slow responding parts of the pancreas.

**[0047]** In an exemplary embodiment, synchronization between islets or within islets is enhanced by providing pharmaceuticals, for example Connexin, to reduce gap resistance. Such pharmaceuticals may be administered, for example, orally, systemically via the blood locally or locally, for example via the bile duct. In an exemplary embodiment of the invention, such pharmaceuticals are provided by genetically altering the cells in the pancreas, for example using genetic engineering methods.

**[0048]** An aspect of some exemplary embodiments relates to implanting electrodes (and/or sensors) in the pancreas. In an exemplary embodiment of the invention, the electrodes are provided via the bile duct. Possibly, a controller, attached to the electrode is also provided via the bile duct. In an exemplary embodiment of the invention, the implantation procedure does not require general anesthesia and is applied using an endoscope. Alternatively, the electrodes are provided through the intestines. Possibly, also the device which controls the electrification of the electrodes is provided through the intestines. In an exemplary embodiment of the invention, the device remains in the intestines, possibly in a folded out portion of the intestines, while the electrodes poke out through the intestines and into the vicinity or the body of the pancreas. Alternatively, the electrodes may be provided through blood vessels, for example the portal vein. In an exemplary embodiment of the invention, the electrodes are elongated electrodes with a plurality of dependent or independent contact points along the electrodes. The electrodes may be straight or curved. In an exemplary embodiment of the invention, the electrodes are poked into the pancreas in a curved manner, for example being guided by the endoscope, so that the electrodes cover a desired surface or volume of the pancreas. The exact coverage may be determined by imaging, or by the detection of the electric field emitted by the electrodes, during a post implantation calibration step.

**[0049]** An aspect of some exemplary embodiments of the invention relates to a pancreatic controller adapted to perform one or more of the above methods. In an exemplary embodiment of the invention, the controller is implantable inside the body. An exemplary controller includes one or more electrodes, a power source for electrifying the electrodes and control circuitry for controlling the electrification. Optionally, a glucose or other sensor is provided for feedback control.

**[0050]** There is thus provided in accordance with an exemplary embodiment of the invention, a pancreatic controller, comprising:

a glucose sensor, for sensing a level of glucose or insulin in a body serum;  
 at least one electrode, for electrifying an insulin producing cell or group of cells;  
 a power source for electrifying said at least one electrode with a pulse that does not initiate an action potential in said cell and has an effect of increasing insulin secretion; and  
 a controller which receives the sensed level and controls said power source to electrify said at least one electrode to have a desired effect on said level. Optionally, said insulin producing cell is contiguous with a pancreas and wherein said electrode is adapted for being placed adjacent said pancreas. Alternatively or additionally, said controller comprises a casing suitable for long term implantation inside the body. Alternatively or additionally, said electrode is adapted for long term contact with bile fluids. Alternatively or additionally, the apparatus comprises an electrical activity sensor for sensing electrical activity of said cell and wherein said power source electrifies said electrode at a frequency higher than a sensed depolarization frequency of said cell, thereby causing said cell to depolarize at the higher frequency.

[0051] In an exemplary embodiment of the invention, said pulse is designed to extend a plateau duration of an action potential of said cell, thereby allowing more calcium inform into the cell. Optionally, said pulse is designed to reduce an action potential frequency of said cell, while not reducing insulin secretion from said cell.

[0052] In an exemplary embodiment of the invention, said pulse is designed to extend a duration of a burst activity of said cell.

[0053] In an exemplary embodiment of the invention, said pulse has an amplitude sufficient to recruit non-participating insulin secreting cells of said group of cells.

[0054] In an exemplary embodiment of the invention, the apparatus comprises at least a second electrode adjacent for electrifying a second cell of group of insulin secreting cells, wherein said controller electrifies said second electrode with a second pulse different from said first electrode. Optionally, said second pulse is designed to suppress insulin secretion. Optionally, said controller is programmed to electrify said second electrode at a later time to forcefully secrete said insulin whose secretion is suppressed earlier. Alternatively, said second pulse is designed to hyper-polarize said second cells.

[0055] In an exemplary embodiment of the invention, said controller electrifies said at least one electrode with a pacing pulse having a sufficient amplitude to force a significant portion of said cells to depolarize, thus aligning the cells' action potentials with respect to the non-excitatory pulse electrification.

[0056] In an exemplary embodiment of the invention, said controller synchronizes the electrification of said electrode to a burst activity of said cell.

[0057] In an exemplary embodiment of the invention, said controller synchronizes the electrification of said electrode to an individual action potential of said cell.

[0058] In an exemplary embodiment of the invention, said controller does not synchronize the electrification of said electrode to electrical activity of said cell.

[0059] In an exemplary embodiment of the invention, said controller does not apply said pulse at every action potential of said cell.

[0060] In an exemplary embodiment of the invention, said controller does not apply said pulse at every burst activity of said cell.

[0061] In an exemplary embodiment of the invention, said pulse has a duration of less than a single action potential of said cell. Optionally, said pulse has a duration of less than a plateau duration of said cell.

[0062] In an exemplary embodiment of the invention, said pulse has a duration of longer than a single action potential of said cell.

[0063] In an exemplary embodiment of the invention, said pulse has a duration of longer than a burst activity duration of said cell.

[0064] In an exemplary embodiment of the invention, said controller determines said electrification in response to a pharmaceutical treatment applied to the cell. Optionally, said pharmaceutical treatment comprises a pancreatic treatment. Alternatively or additionally, said controller applies said pulse to counteract adverse effects of said pharmaceutical treatment.

[0065] In an exemplary embodiment of the invention, said controller applies said pulse to synergistically interact with said pharmaceutical treatment. Alternatively, said controller applies said pulse to counteract adverse effects of pacing stimulation of said cell.

[0066] In an exemplary embodiment of the invention, said apparatus comprises an alert generator. Optionally, said controller activates said alert generator if said glucose level is below a threshold. Alternatively or additionally, said controller activates said alert generator if said glucose level is above a threshold.

[0067] There is also provided a method of controlling insulin secretion, comprising:

providing an electrode to at least a part of a pancreas;  
 applying a non-excitatory pulse to the at least part of a pancreas, which pulse increases secretion of insulin. Optionally, the method comprises applying an excitatory pulse in association with said non-excitatory pulse. Alternatively or additionally, the method comprises applying a secretion reducing non-excitatory in association with said non-excitatory pulse.

[0068] In an exemplary embodiment of the invention, the method comprises applying a plurality of pulses in a sequence designed to achieve a desired effect on said at least a part of a pancreas.

[0069] There is thus provided in accordance with the invention, a pancreatic controller, comprising:

at least one electrode adapted for electrifying at least a portion of a pancreas; and  
a controller programmed to electrify said at least one electrode and adapted to control at least two members of a group consisting of blood glucose level, blood insulin level and blood level of another pancreatic hormone. Optionally, controlling comprises modifying said at least two members simultaneously. Alternatively or additionally, controlling comprises selectively modifying only one of said at least two members, while at least reducing a causative interaction between said two members. Alternatively or additionally, controlling comprises maintaining at least one of said members within a desired physiologic range. Alternatively or additionally, said at least two members comprise glucose level and insulin level. Optionally, controlling comprises modulating an effect of said insulin not related to carbohydrate metabolism.

[0070] In an exemplary embodiment of the invention, at least one of said two members comprise glucagon. Optionally, controlling comprises increasing glucagon secretion, to contract an effect of insulin. Alternatively or additionally, controlling comprises increasing glucagon secretion, to achieve higher blood glucose levels. Alternatively or additionally, controlling comprises reducing the secretion of glucagon, when insulin secretion is increased.

[0071] In an exemplary embodiment of the invention, at least one of said two members comprise Somatostatin. Alternatively or additionally, at least one of said members comprises glucose level. Optionally, said controller selects between alternative control therapies, a therapy that has a least disrupting effect on said glucose levels.

[0072] In an exemplary embodiment of the invention, said controller uses solely electrical fields to control said members.

[0073] In an exemplary embodiment of the invention, said controller takes molecules provided in the body, into account, for said control. Optionally, said molecules are provided without a control of said controller. Alternatively, said molecules are provided under a control of said controller.

[0074] In an exemplary embodiment of the invention, said molecules suppress the secretion of at least one pancreatic hormone. Alternatively or additionally, wherein said molecules suppress the effect of at least one pancreatic hormone. Alternatively or additionally, said molecules enhance the secretion of at least one pancreatic hormone. Alternatively or additionally, said molecules enhance the effect of at least one pancreatic hormone.

[0075] In an exemplary embodiment of the invention,

controlling a member hormone comprises suppressing a secretion of an antagonistic hormone. Alternatively or additionally, controlling a member hormone comprises enhancing a secretion of an antagonistic hormone.

[0076] In an exemplary embodiment of the invention, said controller comprises a learning memory module for storing therein feedback interaction of said pancreas. Optionally, said feedback interactions comprises interactions between hormone levels. Alternatively or additionally, said feedback interactions comprises interactions between hormone levels. Alternatively or additionally, said feedback interactions are dependent on blood glucose levels. Alternatively or additionally, said feedback interactions are determined by said controller, by tracking a behavior of said pancreas. Optionally, said controller actively modifies at least one of a glucose level and a pancreatic hormone level, to collect feedback interaction information.

[0077] In an exemplary embodiment of the invention, the controller comprises a sensor for sensing a level of said controlled member. Alternatively or additionally, the controller comprises an estimator for estimating a level of said controlled member. Alternatively or additionally, said electrode applies a non-excitatory pulse to effect said control. Alternatively or additionally, said electrode applies an excitatory pulse to effect said control.

[0078] In an exemplary embodiment of the invention, said electrode modifies blood flow associated with said pancreas to effect said control. Optionally, said modified blood flow comprises blood flow to hormone generating cells of said pancreas. Alternatively, said modified blood flow comprises blood flow from said pancreas.

[0079] In an exemplary embodiment of the invention, said modified blood flow comprises blood flow from hormone generating cells of said pancreas.

[0080] In an exemplary embodiment of the invention, said at least one electrode comprises at least two electrodes that selectively electrify different parts of said pancreas, to achieve a desired control of said at least two members.

[0081] In an exemplary embodiment of the invention, controlling comprises controlling secretion.

[0082] In an exemplary embodiment of the invention, controlling comprises controlling production. Alternatively or additionally, controlling comprises controlling physiological activity.

[0083] There is also provided a method of mapping pancreatic behavior of a pancreas, comprising:

determining a behavior of a pancreas at a first set of conditions;  
determining a behavior of a pancreas at a second set of conditions; and  
analyzing the behavior of the pancreas and the sets of conditions, to determine a behavior pattern of the pancreas. Optionally, said behavior pattern comprises an interrelationship between two hormones of said pancreas. Alternatively or additionally, said

sets of conditions are naturally occurring. Alternatively, said sets of conditions are at least partially artificially induced.

[0084] In an exemplary embodiment of the invention, the method comprises controlling said pancreas responsive to said determined behavior. Optionally, controlling comprises controlling using pharmaceuticals. Alternatively or additionally, controlling comprises controlling using electrical fields.

## BRIEF DESCRIPTION OF THE DRAWINGS

[0085] Particular embodiments of the invention will be described with reference to the following description of exemplary embodiments in conjunction with the figures, wherein identical structures, elements or parts which appear in more than one figure are optionally labeled with a same or similar number in all the figures in which they appear, in which:

Fig. 1 is a block diagram of a pancreatic controller, in accordance with an exemplary embodiment of the invention;

Fig. 2 is a diagram of an exemplary electrical activity of a single beta cell, operating at slightly elevated glucose levels;

Fig. 3A is a flowchart of an exemplary control logic scheme, in accordance with an exemplary embodiment of the invention;

Fig. 3B is a flowchart of another exemplary control logic scheme, in accordance with an exemplary embodiment of the invention;

Figs. 4A-4D illustrate different types of electrodes that may be suitable for pancreatic electrification, in accordance with exemplary embodiments of the invention;

Fig. 4E illustrates an electrode, in which the body of the controller of Fig. 1 serves as at least one electrode, in accordance with an exemplary embodiment of the invention;

Fig. 5 illustrates a pancreas subdivided into a plurality of control regions, each region being electrified by a different electrode, in accordance with an exemplary embodiment of the invention;

Figs. 6A and 6B are flowcharts of implantation methods, in accordance with exemplary embodiments of the invention;

Fig. 7 is a flowchart of an exemplary method of controller implantation and programming, in accordance with an exemplary embodiment of the invention;

Fig. 8 is a chart showing the effect of electrical stimulation on insulin levels, in six animals;

Fig. 9 is a graphic showing the effect of electrical stimulation on blood glucose levels, in an experiment in which glucose levels are increased faster than would be expected solely by inhibition of insulin

secretion;

Figs. 10A-10B are a chart and a pulse diagram, respectively, of an experiment showing reduction in glucose levels as a result of applying an electrical pulse in accordance with an exemplary embodiment of the invention;

Figs. 11A-11B are a chart and a pulse diagram, respectively, of an experiment showing reduction in glucose levels as a result of applying an electrical pulse in accordance with an exemplary embodiment of the invention;

Figs. 12A-12B are a chart and a pulse diagram, respectively, of an experiment showing reduction in glucose levels as a result of applying an electrical pulse in accordance with an exemplary embodiment of the invention; and

Figs. 13A-13B are a chart and a pulse diagram, respectively, of an experiment showing reduction in glucose levels as a result of applying an electrical pulse in accordance with an exemplary embodiment of the invention.

## DETAILED DESCRIPTION OF EXEMPLARY EMBODIMENTS OVERVIEW

[0086] Fig. 1 is a block diagram of a pancreatic controller 102, in accordance with an exemplary embodiment of the invention. In an exemplary embodiment of the invention, device 102 is used to provide controlling pulses of electricity to a pancreas 100. Such controlling pulses may include excitatory stimulating pulses and non-excitatory pulses. In particular, such pulses can include pacing pulses and action potential modifying pulses.

[0087] In an exemplary embodiment of the invention, the controlling pulses are used to control the glucose and insulin level of a patient. Further, a particular desired profile of glucose and/or insulin may be achieved. Alternatively or additionally, the secretion and/or generation of other pancreatic hormones may be controlled. Other uses of controller 102 will be evident from the description below and can include, for example, training, healing and preventing damage of pancreatic cells.

[0088] Exemplary and non-limiting examples of metabolic and/or hormonal disorders that may be treated by suitable application of the methods described below, include non-insulin dependent diabetes mellitus, insulin dependent diabetes mellitus and hyperinsulemia.

[0089] The following description includes many different pulses that may be applied to achieve a desired effect, it should be clear that the scope of the description also covers apparatus, such as controller 102 that is programmed to apply the pulses and/or process feedback, as required. It should also be noted that a desired effect may be achieved by applying various combinations of the pulses described below, for two different sequences. The particular combinations of pulses that is appropriate for a particular patient may need to be determined on a

patient by patient basis and may also change over time. Exemplary pulses and sequences, however, are described below.

#### EXEMPLARY DEVICE

[0090] Pancreatic controller 102, includes generally a field source 104 for generating electric fields across pancreas 100 or portions thereof, which field source is controlled by control circuitry 106. A power source 108 optionally powers field source 104 and control circuitry 106. The electrification is applied using a plurality of electrodes, for example a common electrode 110 and a plurality of individual electrodes 112. Alternatively other electrode schemes are used, for example a plurality of electrode pairs.

[0091] Electrical and other sensors may be provided as well, for input into controller 106. Although the electrodes may also serve as electrical sensors, in an exemplary embodiment of the invention, separate sensors, such as a pancreatic sensor 114 or a glucose blood sensor 118 on a blood vessel 120, are provided. Extracellular sensors, for measuring inter-cellular glucose levels, may also be provided. Controller 102 may also include an external unit 116, for example for transmitting power or programming to control circuitry 106 and/or power source 108. Alternatively or additionally, the external unit may be used to provide indications from a patient and/or sensor information. Alternatively or additionally, the external unit may be used to provide alerts to the patient, for example if the glucose level is not properly under control. Alternatively or additionally, such alerts may be provided from inside the body, for example using low frequency sounds or by electrical stimulation of a nerve, a muscle or the intestines.

[0092] Additional details of this and other exemplary implementations will be provided below. However, the general structure of controller 102 may utilize elements and design principles used for other electro-physiological controllers, for example as described in PCT publications WO97/25098, WO 98/10831, WO98/10832 and US patent application 09/260,769. It is noted, however, that the frequencies, power levels and duration of pulses in the pancreas may be different from those used, for example, in the heart. In particular, the power levels may be lower. Additionally, the immediate effects of an error in applying a pulse to the pancreas are not expected to be as life threatening as a similar error in the heart would be, excepting the possibility of tissue damage, which would cause an increase in severity of disease of the patient.

#### TISSUE TO WHICH THE CONTROLLER IS APPLIED

[0093] The present invention is described mainly with reference to pancreatic tissues. Such tissue may be in the pancreas or be part of an implant, possibly elsewhere in the body, or even in the controller envelope

itself, the implant comprising, for example, homologous, autologous or heterologous tissue. Alternatively or additionally, the implant may be genetically modified to produce insulin. It should be noted that different parts of the pancreas may have different secretion-related behavior and/or response to electric fields.

#### ELECTRICAL ACTIVITY IN THE PANCREAS

[0094] Fig. 2 is a diagram of an exemplary electrical activity of a single beta cell, operating at slightly elevated glucose levels. In a large scale graph 130, the activity of a single cell is shown as comprising a plurality of burst periods 132 comprising a plurality of individual action potentials and separated by a plurality of interval periods 134, in which periods there are substantially no action potentials. As shown in a blow-up graph 140, each burst comprises a plurality of depolarization events 142, each followed by a repolarization period 144. The level of intracellular calcium increases during the burst 132 and decreases during interval 134.

[0095] The beta cells of a pancreas are arranged in islets, each such islet acts as a single activation domain, in which, when the glucose levels are high enough, a propagating action potential is to be found. Thus, the aggregate electrical activity of an islet is that of a repeating average action potential, at a frequency, of for example, 1 Hz, which generally depends on the propagation time of an action potential through the islet. During intervals 134, if enough of the beta cells share the interval, the entire islet may be generally silent or contain only sporadic depolarization events. Individual cells may operate at higher frequencies, for example, 5-20 Hz. Alternatively or additionally, a slow wave may provide an envelope of about 3-5 cycles/min. It should be noted that the synchronization and/or correlation between cells in an islet may depend on gap junctions between beta and other cells. The resistance or such gap junctions may depend on the glucose and/or hormone levels, and as such, may also be determined and controlled, in accordance with some embodiments of the invention. Alternatively or additionally, the level of synchronization in an islet and/or between islets may be used as an indicator for glucose and/or hormone levels.

#### INSULIN SECRETION INCREASE

[0096] The secretion of insulin, as differentiated from the production of insulin, may be increased in several ways, in accordance with exemplary embodiments of the invention. The following methods may be applied together or separately. Also, these methods may be applied locally, to selected parts of the pancreas, or globally, to the pancreas as a whole.

[0097] In a first method, the duration of a burst 132 is increased, thus allowing more calcium to enter the beta cells. It is believed that the level of calcium in the cell is directly related to the amount of insulin released by the

cell. One type of pulse which may be applied is a pacing pulse, which forces the cells in the islet to depolarize. Such a pulse is optionally applied at the same frequency as individual action potentials, e.g., 10 Hz. However, it may not be necessary to pace every action potential, a periodic pacing signal may be sufficient to force continuous depolarization events. As well known in the art of cardiac pacing, many techniques can be applied to increase the capture probability of the pacing signal, for example, double pacing, pulse shape and duration. These methods may also be applied, with suitable modifications, to the pacing of the pancreas. An alternative method of increasing burst length is by increasing the sensitivity of the beta cells to depolarization, for example, by sub-threshold pulses. Another method of sensitizing the cells and/or increasing their action potential duration is by hyperpolarizing the cells prior to a forced or normal depolarization. Possibly, by preventing the normal reduction in depolarization frequency towards the end of a burst, a higher insulin output can be achieved for a same length burst.

**[0098]** In another method of increasing insulin secretion is by increasing the calcium inflow efficiency of the individual action potentials. In an exemplary embodiment of the invention, this is achieved by increasing the length of the plateau durations 144, for example by applying an electric pulse during the repolarization period associated with each of depolarization events 142. If such a pulse is applied early enough in the repolarization phase of an action potential, period, prior to closing of the calcium channels that provide the calcium inflow, these channels may stay open longer and will provide more calcium inflow. It is noted that the frequency of firing of the beta cells may be reduced.

**[0099]** In some cells, the calcium inflow may be more efficient during the depolarization period. In these cells, depolarization period 142 is optionally extended, for example by applying an additional depolarizing pulse during the depolarization or very shortly after. Alternatively or additionally, a pharmaceutical that enhances repolarization may be provided, so that the repolarization time is shorter and more of the duration of a burst 132 can be spent in depolarization events. Alternatively or additionally, a plateau duration can be shortened by applying a suitable pulse during the plateau. In one example, applying a pulse after the calcium channels close, is expected to shorten the repolarization time. Alternatively or additionally, the individual action potentials are paced, at a rate higher than normal for the glucose level. This pacing can override the end of repolarization and force more frequent depolarization events. It is noted that a considerably higher pacing rate can be achieved by pacing than would naturally occur for same physiological conditions. Possibly, the pacing rate is higher than physiologically normal for an islet at any glucose level.

**[0100]** In another method, the insulin secretion is enhanced by pacing the islets to have a higher frequency

of bursts (as opposed to a higher frequency of action potentials, described above). The resulting shortening in intervals 134 may have undesirable effects, for example by maintaining high calcium levels in a cell for too long a period of time. In an exemplary embodiment of the invention, this potential shortcoming is overcome by increasing the interval durations, for example, by applying a hyper-polarizing pulse during the interval, thus allowing calcium to leak out of the beta cells. It is noted however, that in some cases, sustained elevated calcium levels may be desirable. In which case, the intervals may be artificially shortened. In compensation, the effectiveness of the burst in causing the secretion of insulin may be reduced.

**[0101]** A potential advantage of pacing is that the pacing signal will cause depolarization and associated recruitment of beta cells that would not otherwise take part in the activity of the pancreas. It is expected that as intracellular calcium levels rise (or some other control mechanism), some cells will cease to participate in electrical activity. By applying a pacing pulse, such cells are expected to be forced to participate and, thus, continue to secrete insulin.

**[0102]** Another potential advantage of pacing is related to the synchronization problem. As can be appreciated, some types of controlling pulses need to be applied at a certain phase in the cellular action potential. In a propagating action potential situation, it may be difficult to provide a single pulse with timing that matches all the cells, especially as the depolarization frequency increases. However, by forcing simultaneous depolarization of an entire islet, the phases are synchronized, making a desirable pulse timing easier to achieve. It is noted, however, that even if there is no pacing, some pulses, such as for extending a plateau of an action potentials, can be applied at a time that is effective for a large fraction of the cells in the islet.

**[0103]** Alternatively or additionally to calcium mediated vesicle transport, in an exemplary embodiment of the invention, the electrical field also directly releases insulin from the REP of the cell and/or from other organelles in the cell.

## INSULIN SECRETION SUPPRESSION

**[0104]** In some cases, for example if the glucose level is too low, suppression of insulin secretion may be desirable. Again, the following methods may be applied together or separately. Also, as noted above, different methods may be applied to different parts of the pancreas, for example, by differently electrifying electrodes 112 of Fig. 1, thus for example, increasing secretion from one part of the pancreas while decreasing secretion from a different part at the same time.

**[0105]** In a first method of insulin secretion reduction, the beta cells are hyper polarized, for example by applying a DC pulse. Thus, the cells will not respond to elevated glucose levels by depolarization and insulin se-

cretion. It is noted that the applied pulse does not need to be synchronized to the electrical activity. It is expected that the hyper polarization will last a short while after the pulse is terminated. Possibly, only the length of the interval is increased, instead of completely stopping the burst activity.

[0106] In a second method, the insulin stores of the pancreas are dumped, so that at later times, the cells will not have significant amounts of insulin available for secretion. Such dumping may be performed for example, with simultaneous provision of glucose or an insulin antagonist, to prevent adverse effects. The insulin antagonist, glucose or other pharmaceuticals described herein may be provided in many ways. However, in an exemplary embodiment of the invention, they are provided by external unit 116 or by an internal pump (not shown) in controller 102.

[0107] In a third method, the plateau durations are shortened, for example by over-pacing the islet cells, so that there is less available time for calcium inflow. Alternatively, the intra-depolarization periods may be extended, by hyper-polarizing the cells during repolarization and after the calcium channels close (or forcing them closed by the hyper polarization). This hyper polarization will delay the onset of the next depolarization and thus, reduce the total inflow of calcium over a period of time.

[0108] Alternatively or additionally, a hyper-polarizing pulse may be applied during a burst, to shorten the burst.

#### AFFECTING INSULIN PRODUCTION

[0109] Various feedback mechanisms are believed to link the electrical activity of the beta cells and the production of insulin. In an exemplary embodiment of the invention, these feedback mechanisms are manipulated to increase or decrease insulin production, alternatively or additionally to directly controlling insulin secretion.

[0110] In an exemplary embodiment of the invention, beta cells are prevented from secreting insulin, for example, by applying a hyper-polarizing pulse. Thus, the intra-cellular stores remain full and less insulin is manufactured (and thus less insulin can reach the blood stream).

[0111] In an exemplary embodiment of the invention, the beta cells are stimulated to release insulin. Depending on the cell, it is expected that if a cell is over stimulated, it becomes tired out and requires a significant amount of time to recover, during which time it does not produce insulin. If a cell is under stimulated, it is expected that it will, over time produce less insulin, as it adapts to its new conditions. If a cell is stimulated enough, it will continuously produce insulin at a maximal rate.

#### PANCREATIC RESPONSE CONTROL

[0112] In an exemplary embodiment of the invention,

rather than directly control insulin secretion levels, the response parameters of the pancreas are modified, to respond differently to glucose levels. One parameter that may be varied is the response time. Another parameter is the gain (amplitude) of the response. In some situations, these two parameters cannot be separated. However, it is noted that by providing complete control of the pancreas, many different response profiles can be provided by controller 102 directly.

[0113] In an exemplary embodiment of the invention, the response time of the pancreas is increased or reduced by blocking or priming the fast-responding portions of the pancreas, in patients that have both fast and slow responding portions. Blocking may be achieved, for example, by partial or complete hyper-polarization. Priming may be achieved, for example, by applying a sub-threshold pulse, for example, just before depolarization. A potential advantage of such a sub-threshold pulse is that it may use less power than other pulses.

[0114] The gain of the response may be controlled, for example, by blocking or by priming parts of the pancreas, to control the total amount of pancreatic tissue taking part in the response. It is noted that priming "slow response" cells causes them to act as fast response cells, thereby increasing the gain of the fast response. In some cases, the priming and/or blocking may need to be repeated periodically, to maintain the sensitivity profile of the pancreas as described.

[0115] Alternatively or additionally, the sensitivity of the pancreas may be enhanced (or decreased) by supporting (or preventing) the propagation of action potentials, for example by providing a suitable pharmaceutical. Octonal and Heptonal are examples of pharmaceuticals that decouple gap junctions.

[0116] In an alternative embodiment of the invention, the secretion and/or production ability of part or all of the pancreas is modified, by controlling the blood flow to and/or from the pancreas.

[0117] It is hypothesized that reducing the blood flow to the pancreas will reduce the production and/or secretion rate of various pancreatic hormones.

[0118] Alternatively or additionally, by preventing hormone laden blood from leaving the pancreas, the local concentration of the various hormones increases and exhibits a stronger secretion enhancing or inhibiting effect (as the case may be) for other hormones.

#### NON-INSULIN CONTROL

[0119] Alternatively or additionally to controlling the secretion or production of insulin, the secretion and/or production of other pancreatic hormones may be controlled. Exemplary such hormones include glucagon, somatostatin and pancreatic poly-peptide (PP). The levels and/or profile of level of these hormones may be controlled while controlling insulin levels or while ignoring insulin levels. In some embodiments of the invention, the hormones may be controlled partially independently

of insulin.

[0120] Some of the pancreatic hormones interact via biological feedback mechanisms, for example, an increase in glucagon also increases insulin. These interactions may be represented using a set of equations. In other embodiments, a neural network may be used. In an exemplary embodiment of the invention, use is made of the fact that the feedback equations are not linear. Instead, the equations typically include a time delay and different gains for different relative hormonal levels. Further, the physiological mechanism may depend on glucose levels, on nervous stimulation, on previous activity of the pancreas and/or on various digestive hormone. The particular equations and/or equation parameter for a particular patient may need to be determined for that patient, for example by controlled experimentation (e.g., modifying one hormonal level and tracking the effect on others) or by observation.

[0121] Once the equations are known, the control of one hormone may be independent of other hormones. For example, instead of providing a large increase in glucagon, which will increase insulin levels, a smaller increase, over a long period of time, may have a similar effect, without prompting glucagon secretion (which would confound the glucose lowering effect of the insulin). Alternatively or additionally, the increase in glucagon (or, conversely, insulin or other pancreatic hormones) is made as a series of short bursts, with rest periods between bursts. Thus, even though the secreted hormone performs its activity, it does not build up in the blood and/or in the pancreatic cells, to levels which will cause significant secretion of the antagonistic hormone.

[0122] Alternatively or additionally, pharmaceuticals may be used to reduce the sensitivity of one cell type relative to other cell types (or to increase the sensitivity), thus modifying the feedback equations and allowing some leeway in selective control of the hormones. Alternatively, the responses of the cells may be regularized by the pharmaceuticals, so all cell types respond in a more uniform manner. Exemplary pharmaceuticals that selectively affect pancreatic behavior, include streptozotocin and alloxan, which reduce insulin output from beta-cells and various drugs used for treatment of diabetes.

[0123] Alternatively or additionally, the pharmaceuticals that are provided block the receptors for the hormone to be selectively disabled. Alternatively or additionally, the pharmaceuticals, for example antibodies, disable the hormone in the blood stream.

[0124] Exemplary pharmaceuticals are described, for example, in *J Biol Chem* 2000 Feb 11; 275(6):3827-37, *Acta Crystallogr D Biol Crystallogr* 2000 May; 56 (Pt 5): 573-80, *Metabolism* 1999 Jun; 48(6):716-24, *Am J Physiol* 1999 Jan; 276(1 Pt 1):E19-24, *Endocrinology* 1998 Nov; 139(11):4448-54, *FEBS Lett* 2000 May 12; 473(2):207-11, *Am J Physiol* 1999 Aug; 277(2 Pt 1): E283-90, *Cur Pharm Des* 1999 Apr; 5(4):255-63 and *J*

*Clin Invest* 19998 Apr 1;101(7):1421-30.

[0125] Alternatively or additionally, as different parts of the pancreas have different ratios of cell types, differential modification of one hormone over other hormones may be achieved by selectively stimulating only certain pancreas portions and/or selectively blocking the activity of pancreas portions.

[0126] Alternatively or additionally, the response of different cell types to a same electrical field stimulation may be different, thus allowing differential control of different hormones.

[0127] A distinction should be noted between controlling hormonal levels and controlling glucose levels by causing the secretion of hormones. Glucose level control at least prevents the damage to the body cause by high or low glucose levels, however, it does not guarantee the availability of glucose to the body cells. Maintaining desirable hormone levels, on the other hand, can not only maintain glucose within a desired range, it can also guarantee that a sufficient level of insulin is available so the body cells can assimilate the glucose. Additionally, various desirable bodily effects caused by the hormones, such as control of fat and protein metabolism or prevention of insulin tolerance, can be achieved.

[0128] It should be noted, that in some cases what is desirable is a hormone ratio or a temporal hormone profile, rather than a simple hormonal value. These effects can be achieved, for example, by temporally varying the control of the hormones.

## EXEMPLARY CONTROL LOGIC

[0129] Fig. 3A is a flowchart of an exemplary control logic scheme 200, in accordance with an exemplary embodiment of the invention. In this scheme, the intensity of pancreatic activity (and associated dangers) is increased with the increase in glucose level. The various methods of increasing and decreasing pancreatic activity are described in more detail above or below. Alerts are optionally provided to the patient at extreme glucose levels. In addition, the method possibly prefers to error on the side of causing hyperglycemia, whose adverse effects are less critical than those of hypoglycemia, whose adverse effects are immediate. It is noted that automated control logic for controlling glucose levels have been developed previously for insulin pumps and may also be applied for controller 102. An added ability of controller 102 is to suppress the body's own production of Insulin. An added limitation which controller 102 optionally takes into account is the avoidance of damaging the pancreas by over stimulation.

[0130] In a step 202, the glucose level is determined. Many methods may be used to determine glucose level. In an exemplary embodiment of the invention, in cases of hyperglycemia, the measurement is repeated several times before starting treatment. In cases of hypoglycemia, the measurements may be repeated few times or not at all, before starting treatment. The cycle of treat-

ment is optionally repeated every two to five minutes. Alternatively, in critical situations such as hypoglycemia, the cycle is repeated even more frequently.

[0131] If the glucose level is under 60 (mg/dl) (step 204), further insulin production is optionally suppressed (206) and, optionally, the patient is alerted (208).

[0132] If the glucose level is between 60 and 150 (210), no action is taken, as these are normal glucose levels.

[0133] If the glucose level is between 150 and 200 (212), the action taken depends on the previous action taken and the previous measured glucose level. If, for example the previous level was higher, the insulin secretion activity may be maintained or reduced. If, on the other hand the glucose level was lower, the insulin secretion level may be increased. For example, a pulse application ratio of 1:3 between burst that are modified and bursts that are not modified may be provided if the glucose level is now reduced from its previous measurement. It should be appreciated, of course that the exact glucose levels and pulse parameters used for a particular patient will depend only on the patient's medical history, but also on that patient's particular response to the pulse parameters used. Some patients may not respond as well as other patients and a more powerful pancreatic activity modification schedule used.

[0134] If the glucose level is between 200 and 250 (216), the action taken (218) can depend on the previous action taken for example providing a pulse application ratio between 1:1 and 1:2. Alternatively or additionally, the action taken can depend on the degree of change, direction of change and/or rate of change of glucose levels. Optionally, a model of insulin secretion, digestion and/or effect on blood glucose level are used to assess the significance of changes in glucose level.

[0135] If the glucose level is between 250 and 300 (220), an even higher pulse application rate, such as 1:1, can be applied (222).

[0136] Glucose levels higher than 300 can be quite dangerous. Thus, if such high rates are determined, a faster pacing rate, to the burst or to the individual action potentials (224), may be applied. Alternatively or additionally, a non-excitatory pulse to enhance secretion is also applied to at least some of the pacing pulses.

[0137] If the level is over 400 (226), a bi-phasic pacing pulse for the individual action potentials (228) may be provided. Such a pulse is expected at its first phase to induce depolarization and at its second phase to extend a plateau duration such that calcium inflow is increased. Alternatively or additionally, if not previously applied, control of multiple pancreatic regions may be provided, to increase the total portion of the pancreas being used to secrete insulin at a higher rate.

[0138] If the glucose level is over 500 (230) emergency measures may be required, for example alerting the patient or his physician (232) and dumping all available insulin in the pancreas (234). A store of available insulin may be maintained in the pancreas or in device 102 (or

an associated insulin pump) for just these cases.

[0139] It should be noted the above method is only exemplary. For example, the exact action at each may be modified, as can be the mixture of actions, the pulse parameters and the delays before changing action.

[0140] This control method utilizes delayed closed loop control circuits. Alternatively, open-loop circuits, which are similar to conventional glucose level management, may be provided. In such a loop, the amount of insulin output from a particular pulse application is known and is applied responsive to an infrequent measurement of the glucose level, for example using a blood test. Periodic glucose level testing may be applied to detect failed control. Intermediate control loops, control circuits having a smaller delay and combined control loops (having both open loop and closed loop) may be used in other exemplary embodiments of the invention.

## LONG TERM AND SHORT TERM CONSIDERATIONS

[0141] When applying electrification pulses in accordance with exemplary embodiments of the invention, both short term and long term effects are optionally taken into considerations. Short term effects, include, for example effects on of insulin secretion and production. Long term effects include, for example, effects on tissue viability and capability and electrode polarization.

[0142] As will be described below, long terms effects may be negative, such as cell death, or positive, such as training or promoting healing.

[0143] Polarization and encrustation of the electrodes are optionally avoided by using ionic electrodes and applying balanced pulses (with substantially equal positive and negative charges). Alternatively, special coated electrodes, such as those coated with Iridium oxide or titanium nitride, may be used. Alternatively or additionally, relatively large electrodes may be used. The balancing may be on a per pulse basis or may be spread over several pulses.

[0144] In an exemplary embodiment of the invention, controller 102 stores in a memory associated therewith (not shown) a recording of the glucose levels, the applied electrical and/or pharmaceutical control, food intake and/or the effect of the applied control on electrical activity of the pancreas and/or effects on the blood glucose level.

## CELLULAR TRAINING

[0145] In an exemplary embodiment of the invention, the applied electrification and/or pharmaceutical profiles are used to modify the behavior of islet cells, in essence, training the cells to adapt to certain conditions. It is expected that slightly stressing a beta cell will cause the cell to compensate, for example by enlarging or by causing new beta cells to be produced. Such regeneration mechanism are known to exist, for example as described in "Amelioration of Diabetes Mellitus in partially

Depancreatized Rats by poly(ADP-ribose) synthetase inhibitors. Evidence of Islet B-cell Regeneration", by Y Yonemura et. al, in *Diabetes*, 33(4):401-404, April 1984. Over stressing can kill the cell. Thus, the level of stress that enhances the cells' operation may need to be determined by trial and error for each patient. In an exemplary embodiment of the invention, the trial and errors are performed on different parts of the pancreas, optionally with a bias to under-stressing rather than for over stressing. In an exemplary embodiment of the invention, over stressing is determined by a marked reduction in insulin output or by reduced or abnormal electrical response.

[0146] Alternatively or additionally, a pancreatic cell insensitive to medium glucose levels may be trained to be sensitive to lower glucose level, by exciting it more frequently and/or exciting it at times of slightly elevated glucose levels.

[0147] In an exemplary embodiment of the invention, such training pulses are applied in combination with pharmaceuticals aimed to cause regeneration or healing.

[0148] It is noted that training and activation profile matching can also be used to maintain a cell in shape in a patient temporarily taking insulin, or to support a cell that is recuperating, for example from a toxic material or from the onset of diabetes.

#### ADDITIONAL EXEMPLARY LOGIC

[0149] Fig. 3B is a flowchart of another exemplary control logic scheme 240, in accordance with an exemplary embodiment of the invention. Fig. 3B is similar to Fig. 3A, however, a lower degree of discrimination between glucose levels is shown in Fig. 3B, for clarity presentation. The reference numbers in Fig. 3B are 40 more than for corresponding elements in Fig. 3A.

[0150] Fig. 3B illustrates controlling hormonal levels, increasing glucagon secretion and selecting a treatment protocol or parameter based on the effect on pancreatic hormones other than insulin.

[0151] In response to a glucose level sensing (242), if the level is low, presenting hypoglycemia, insulin secretion is optionally suppressed (246). Alternatively or additionally, glucagon secretion is increased (245).

[0152] If the glucose levels are normal (250), an additional test is optionally performed, as to whether the hormonal levels are normal (251). In an exemplary embodiment of the invention, the hormone levels (e.g., insulin and/or glucagon) are directly measured using suitable sensors, for example fiber optic sensors or limited use chemical assay sensors. Alternatively or additionally, the levels are estimated based on the variation in blood glucose levels and/or electrical activity of the pancreas. If hormone levels are too low, they are increased (253). Possibly, if the hormone levels are too high, stimulation is stopped and/or even suppressed (not shown). Possibly, a control logic similar to that of Figs. 3A and

3B is prompted by a sensing of hormone levels.

[0153] Skipping elements 252 through 258, which are the same as in Fig. 3A, if the glucose level is high and a fast response is desired, a test is made as to which one of a plurality of available treatments and/or treatment parameters is preferred (260). One issue is which treatment will cause the secretion of glucagon, which secretion will confound the desired glucose reducing effect.

[0154] In any case, if after a suitable time delay the glucose levels have not gone down (266) more drastic treatment is applied.

#### PULSE SHAPES AND PARAMETERS

[0155] The range of pulse forms that may be applied usefully is very wide. It must be noted that the response of the cells in different patients or of different cells in a same patient, even to same pulses, is expected to differ considerably, for example due to genetics and disease state. Also, the conduction of electrical signals in the vicinity of the pancreas is affected by the irregular geometrical form of the pancreas and the layers of fat surrounding it. These isolating layers may require the application of higher than expected amplitudes.

[0156] It is also noted that, at least for some embodiments, the application of the pulse is for affecting a certain portion of the pancreas and not the entire pancreas.

[0157] The lack of significant propagation of action potentials from one islet of the pancreas to another may require a relatively uniform field in the part of the pancreas to be affected. However, completely uniform fields are not required as any edge effects are contained only to the islets with the intermediate electric field strengths and/or because it is expected that the cell behavior does not vary sharply with the applied amplitude, except perhaps at certain threshold levels.

[0158] Further, the beta cells' behavior may be dependent on glucose level, on cellular insulin storage level and/or on previous activity of the cells. Unlike cardiac cells, which operate continuously and typically at a limit of their ability and/or oxygen usage, normal pancreatic cells are provided with long rests and are operated at sub-maximal levels.

[0159] A first parameter of the pulse is whether it is AC or DC. As the pulse may be applied periodically, the term DC pulse is used for a pulse that does not alternate in amplitude considerably during a single application, while an AC pulse does, for example having an intrinsic frequency an order of magnitude greater than 1/pulse duration. In an exemplary embodiment of the invention, DC pulses or pulses having a small number of cycles per application, are used. In this usage, a pulse that is synchronized to a burst is considered AC if it alternates in amplitude, for example ten times over the burst duration, even though this frequency is actually lower than the action potential frequency. If, conversely, the pulse is a square pulse synchronized to the individual action

potentials, it will be considered a DC pulse, for this discussion, although its actual frequency is higher than the AC pulse.

**[0160]** Exemplary frequencies for AC pulses applied to bursts are between 1 and 1000 Hz and for AC pulses applied to action potentials, between 20 and 2000 Hz. Optionally, the AC frequencies are between 50 and 150 Hz.

**[0161]** Various pulse durations may be used. An advantage of a DC long duration pulse is the lack of transients that might inadvertently affect other tissue. Such a pulse is expected to be useful for hyper-polarization of cells and, thus, may last for several seconds or even minutes or hours. Optionally however, very long duration pulses are interrupted and possibly, their polarity switched to prevent adverse effects such as tissue polarization near the electrodes or over-polarization of the target tissue.

**[0162]** A pulse for affecting a burst may last, for example, between 1 ms and 100 seconds. Exemplary durations are 10 ms, 100 ms and 0.5 seconds. Long pulses may be, for example 2 or 20 seconds long. A pulse for affecting a single action potential will generally be considerably shorter, for example being between 10 and 500 ms long. Exemplary durations are 20, 50 and 100 ms. However, longer pulses, such as 600 or 6000 ms long may also be applied.

**[0163]** In AC pulses, various duty cycles can be used, for example 10%, 50%, 90% and 100%. The percentages may reflect the on/off time of the pulse or they may reflect the relative charge densities during the on and off times. For example, a 50% duty cycle may be providing, on the average, 50% of the maximum charge flow of the pulse.

**[0164]** A pulse may be unipolar or bipolar. In an exemplary embodiment of the invention, balanced pulses, having a total of zero charge transfer, are used. Alternatively, however, the balancing may also be achieved over a train of pulses or over a longer period. It is expected that at least for some pulse effects, the islets will act independently of the polarity of the applied pulse. However, changes in polarity may still have desirable effects, for example by creating ionic current.

**[0165]** Different pulse envelopes are known to interact with cell membranes in different ways. The pulse envelope may be, for example, sinusoid, triangular, square, exponential decaying, bi-phasic or sigmoid. The pulse may be symmetric or asymmetric. Optionally, the pulse envelope is selected to take into account variations in tissue impedance during the pulse application and/or efficiency and/or simplicity of the power electronics.

**[0166]** In an exemplary embodiment of the invention, the pulse current is controlled, for example to remain within a range. Alternatively or additionally, the pulse voltage is controlled, for example to remain within a range. Alternatively or additionally, both current and voltage are at least partly controlled, for example main-

tained in certain ranges. Possibly, a pulse is defined by its total charge.

**[0167]** Different types of pulses will generally, but not necessarily, have different amplitudes. The different effects of the pulse may also be a function of the cell activity phase and especially the sensitivity of the cell to electric fields at the time of application. Exemplary pulse amplitude types are sub-threshold pulses that affect the depolarization state of the cell and channel affecting pulses. These pulses are non-limiting examples of non-excitatory pulses, which do not cause a propagating action potential in the islet, either because of absolute low amplitude or due to relative low amplitude (relative to cell sensitivity). An islet current of 5 pA is suggested in the Medtronic PCT publication, for stimulating pulses.

**[0168]** Pacing pulses definitely cause a propagating action potential, unless the pacing pulse captures all the cells in the islet, in which case there may be nowhere for the action potential to propagate to.

**[0169]** "Defibrillation" pulses are stronger than pacing pulses and cause a rest in the electrical state of the affected cells.

**[0170]** Pore forming pulses, for example high voltage pulses, create pores in the membrane of the affected cells, allowing calcium to leak in or out and/or allowing insulin to leak out.

**[0171]** The above pulse types were listed in order of increasing typical amplitude. Exemplary amplitudes depend on many factors, as noted above. However, an exemplary pacing pulse is between 1 and 20 mA. An exemplary non-excitatory pulse is between 1 and 7 mA. A sub-threshold pulse may be, for example, between 0.1 and 0.5 mA. It is noted that the lack of excitation may be due to the timing of application of the pulse.

**[0172]** Simple pulse forms can be combined to form complex pulse shapes and especially to form pulse trains. One example of a pulse train is a double pacing pulse (two pulses separated by a 20 ms delay) to ensure capture of a pacing signal.

**[0173]** Another example of a pulse train is a pacing pulse followed, at a short delay, by a plateau extending pulse and/or other action potential control pulses. Thus, not only is pacing forced, possibly at a higher than normal rate, but also the effectiveness of each action potential is increased. The delay between the pacing pulse and the action potential control pulse can depend, for example, in the shape of the action potential and especially on the timing of opening and closing of the different ionic channels and pumps. Exemplary delays are 10, 50, 200 and 400 ms.

**[0174]** In some embodiments of the invention a graded pulse is applied. A first part of the pulse blocks first cells from responding to a second part of the pulse. Such a pulse may be used, for example, to differentiate between different cell types, between cells having different stimulation levels and/or between cells having a fast response and cells having a slow response. The exact behavior of such a pulse and/or suitable parameters may

be determined during a training stage, described with reference to Fig. 7, below.

## PULSE TIMINGS

[0175] Not only are various pulse forms contemplated, also different variations in their periodicity are contemplated.

[0176] A first consideration is whether to synchronize an excitatory and/or a non-excitatory pulse to the pancreatic activity or not. If the pulse is synchronized, it can be synchronized to the activity of particular cells or islets being measured. As noted above, a pacing pulse to the pancreas can force synchronization. The pulse may be synchronized to individual action potentials and/or to burst activity. Within an action potential, the pulse can be synchronized to different features of the action potential, for example the depolarization, plateau, repolarization and quiescent period before depolarization. Not all action potentials will exhibit exactly those features.

[0177] Within a burst, a pulse may be synchronized to the start or end of the burst or to changes in the burst envelope, for example, significant reductions in the action potential frequency or amplitude.

[0178] As used herein, synchronization to an event includes being applied at a delay relative to the event occurring or at a delay to when the event is expected to occur (positive or negative delay). Such a delay can be constant or can vary, for example being dependent on the action potential or the burst activity.

[0179] The pulse may be applied at every event to which it is synchronized for example every action potential or every burst. Alternatively, pulses are applied to fewer than all events, for example at a ratio of 1:2, 1:3, 1:10 or 1:20. An exemplary reason for reducing the pulse application ratio is to prevent overstressing the beta cells and causing cellular degeneration, or to provide finer control over secretion rate.

[0180] In some pulses, a significant parameter is the frequency of application of the pulse (as differentiated from the frequency of amplitude variations in a single pulse). Exemplary frequencies range from 0.1 Hz to 100 Hz, depending on the type of pulse.

[0181] In an exemplary embodiment of the invention, the pulse parameters depend on the islet or cellular electrical and/or physiological state. Such a state may be determined, for example using suitable sensors or may be estimated from a global state of the glucose level.

## SENSORS

[0182] Many types of sensors may be usefully applied towards providing feedback for controller 102, including, for example:

(a) Glucose sensors, for example for determining the actual glucose level and providing feedback on

the effects of the pancreatic treatment. Thus, for example, in a patient with weakened pancreatic response, the pancreas will be stimulated to secrete more insulin when the glucose levels are too high. Many types of glucose sensors are known in the art and may be used for the purposes of the present invention, including, for example optical, chemical, ultrasonic, heart rate, biologic (e.g., encapsulated beta cells) and electric (tracking beta cell and/or islet electrical behavior). These sensors may be inside the body or outside of it., connected to controller 102 by wired or wireless means, be in contact with the blood or outside of blood vessels.

(b) Digestion sensors, for example for detecting the ingestion- or upcoming intake- of meals, and, for example, prompting the production of insulin or increase in cell sensitivity. Many suitable sensors are known in the art, for example impedance sensors that measure the stomach impedance, acceleration sensors that measure stomach or intestines movements and electrical sensors that measure electrical activity. Digestion sensing cells are inherently problematic if they do not provide a measure of glucose actually ingested. Optionally, they are used in combination with other sensors and/or only if the digestion system is activated in a profile matching eating, for example a long duration activation or activation that advances along the digestive system. In an exemplary embodiment of the invention, stimulation during the digestion may be stopped, to at least some parts of the pancreas (e.g., ones comprising fewer islets), to avoid interfering with other cell types in the pancreas, for example those that produce digestive juices. Alternatively or additionally, the application of stimulation in general may be optimized to reduce interaction with non-beta cells, for example alpha cells. As alpha cells generate glucagon, their stimulation may be determined by tracking serum glucagon levels.

(c) Pancreatic activity sensors, for example electrodes coupled to the entire pancreas, small parts of it, individual islet(s) or individual cell(s) in an islet. Such sensors are useful not only for providing feedback on the activity of the pancreas and whether the applied pulses had a desired electrical (as opposed to glucose-) effect, but also for synchronizing to the pancreatic electrical activity.

(d) Calcium sensors, both for intracellular spaces and for extra-cellular spaces. As can be appreciated, measuring calcium inside a cell may affect the behavior of the cell. In an exemplary embodiment of the invention, only one or a few cells are used as a sample for the state of the other cells. An exemplary method of intracellular calcium measurement is to stain the cell with a calcium sensitive dye and track its optical characteristics. It is noted that both intra- and extra- cellular calcium levels may affect the electrical and secretory activity of beta cells.

(e) Insulin sensors, of any type known in the art may be used to measure the response of a single islet, the pancreas as a whole and/or to determine blood levels of insulin.

(f) Sensors for other pancreatic hormones, for example, for glucagon and/or Somatostatin. As will be mentioned below, in some cases the levels various pancreatic hormones may be estimated based on changes in blood glucose levels, which changes correspond to previously observed changes during which the hormone levels were measured.

**[0183]** The measurements of the above sensors are optionally used to modify the pulse parameters or pulse application regime. Alternatively or additionally, the sensors are used to track the response to the regime and/or lack of application of pulses, or for calibration.

**[0184]** Different sensing regiments may be use, including continuous sensing, and periodic sensing. Some sensors may provide a frequent measurement, for example every few seconds or minutes. Other sensors may be considerably slower, for example taking a measurement every ten minutes or hour. If only a periodic measurement is required, the measurement may be an average over the time between measurements or it may be an average over a shorter time or an instantaneous value. In some cases a long term integrative sensing, for example of total insulin production, is desirable. A one-time chemical sensor may be suitable for such integrative sensing.

#### TYPES OF ELECTRODES

**[0185]** The electrodes used may be single functionality electrodes, for example only for pacing or only for non-excitatory pulses. Also, different types of non-excitatory pulses, such as hyper-polarization and plateau extension pulses, may use different types of electrode geometries. Alternatively, a combination electrode, comprising both a pacing portion and a pulse application portion, may be provided. The different types of electrodes may have different shapes, for example due to the pacing electrode being designed for efficiency and the pulse electrode being designed for field uniformity. The two electrode functions may share a same lead or they may use different leads. Alternatively, a single electrode form is used for both pacing and non-excitatory pulse application.

**[0186]** Figs. 4A-4D illustrate different types of electrodes that may be suitable for pancreatic electrification, in accordance with exemplary embodiments of the invention.

**[0187]** Fig. 4A illustrates a point electrode 300 having a single electrical contact area at a tip 304 of a lead 302 thereof.

**[0188]** Fig. 4B illustrates a line electrode 306 having a plurality of electric contacts 310 along a length of a lead 308 thereof. An advantage of wire and point elec-

trode is an expected ease in implantation using endoscopic and/or other minimally invasive techniques. In an exemplary embodiment of the invention, multiple wire electrodes are implanted.

**[0189]** Fig. 4C illustrates a mesh electrode 312, including a lead 314 and having a plurality of contact points 318 at meeting points of mesh wires 316. Alternatively or additionally, some of the wire segments between meeting points provide elongate electrical contacts.

**[0190]** Each of the contact points can be made small, for example slightly larger than an islet. Alternatively, larger contact areas are used. In line electrodes, exemplary contact areas are 0.2, 0.5, 1, 2 or 5 mm long. In some embodiments of the invention, smaller contact areas than used for cardiac pacemakers may be suitable, as smaller fields may be sufficient.

**[0191]** In some embodiments, volume excitation of the pancreas is desired. Fig. 4D illustrates various volume excitation electrodes. A plate electrode 320 includes a plate 322 that can simultaneously excite a large area. A ball electrode 324 includes a ball shaped contact area 326, with a radius of, for example, 2 or 4 mm, for exciting tissue surrounding ball 326. A hollow volume electrode 328, for example, includes an open volume contact area 330, for example a mesh ball or a goblet, which can be used to excite tissue in contact with any part of ball 330, including its interior. Another possibility is a coil electrode. Optionally, the coils have a significant radius, such as 2 or 5 mm, so they enclose significant pancreatic tissue. It is noted that volume (and other electrodes as well) electrodes may encompass a small or large part of the pancreas or even be situated to electrify substantially all the insulin producing parts of the pancreas.

**[0192]** Any of the above electrodes can be unipolar or bipolar. In bipolar embodiments, a single contact area may be split or the bi-polar activity may be exhibited between adjacent contact points.

**[0193]** In addition, the above multi-contact point electrodes may have all the contact points shorted together. Alternatively, at least some of the contact points can be electrified separately and, optionally, independently, of other contact points in a same electrode.

**[0194]** Electrical contact between an electrode and the pancreas can be enhanced in many ways, for example using porous electrode, steroids (especially by using steroid eluting electrodes) and/or other techniques known in the art. The type of electrode may be any of those known in the art and especially those designed for long term electrical stimulation.

**[0195]** Fig. 4E illustrates a different type of electrode, in which a casing 332 of controller 102 serves as one or multiple electrodes. Casing 332 may be concave, convex or have a more complex geometry. Possibly, no external electrodes outside of casing 332 are used. Optionally, casing 332 is then made concave, to receive the pancreas. Alternatively, at least a common electrode

336 outside of controller 102 is provided. Alternatively or additionally, casing 332 of controller 102 serves as a common electrode. In an exemplary embodiment of the invention, a plurality of electrodes 334 are formed in casing 332. The electrode types can be any of those described above, for example. Optionally, but not necessarily, electrodes 334 stick out of casing 332. In an exemplary embodiment of the invention, controller 102 is placed in contact with pancreas 100, as an electrically insulating layer of fat usually encapsulates the pancreas. Optionally, the geometry of casing 332 is made to conform to the shape of the pancreas, thus assuring contact with the pancreas and minimal trauma to the pancreas by the implantation. Optionally, a flexible or multi-part hinged casing is provided, to better conform the casing to the pancreas.

[0196] The electrodes can be fixed to the pancreas in many means, including, for example, using one or more sutures or clips, providing coils or roughness in the electrode body, using adhesive or by impaling the pancreas or nearby tissue. An electrode may include a loop, a hole or other structure in it for fixing the suture or clip thereto. It is noted that the pancreas does not move around as much as the heart, so less resilient electrode and lead materials and attachment methods may be used.

[0197] Various combinations of the above electrodes may be used in a single device, for example a combination of a mesh electrode underneath the pancreas and a ground needle electrode above the pancreas. Such a ground electrode may also be inserted in nearby structures, such as the abdominal muscles.

[0198] As described below, the pancreas may be controlled as plurality of controlled regions. A single electrode may be shared between several regions. Alternatively or additionally, a plurality of different electrodes may be provided for the different regions or even for a single region.

#### PANCREATIC CONTROL REGIONS

[0199] Fig. 5 illustrates a pancreas subdivided into a plurality of control regions 340, each region being electrified by a different electrode 342. Control regions 340 may overlap (as shown) or they may be none-overlapping. Possibly, the entire pancreas is also a control region, for example for insulin secretion suppression. Although a significant percentage of the pancreas is optionally controlled, for example 10%, 20%, 40% or 60%, part of the pancreas may remain uncontrolled, for example as a control region or as a safety measure. The number of control regions can vary, being for example, two, three, four, six or even ten or more.

[0200] One possible of different control regions is to allow one part of the pancreas to rest while another part is being stimulated to exert itself. Another possible use is for testing different treatment protocols on different regions. Another possible use is to provide different control logic for parts of the pancreas with different capabilities,

to better utilize those regions or to prevent damage to those regions. For example, different pulses may be applied to fast responding or slow responding portions. In addition, some parts of the pancreas may be more diseased than other parts.

[0201] Optionally, the density and/or size of the electrodes placement on the pancreas (and independently controllable parts of the electrodes) varies and is dependent, for example, on the distribution and density of islet cells in the pancreas. For example, a more densely populated section of the pancreas may be provided with finer electrical control. It is noted that the distribution may be the original distribution or may be the distribution after the pancreas is diseased and some of the cells died or were damaged.

[0202] As noted above, different parts of the pancreas may produce different types and/or relative amounts of various hormones. Thus, selective spatial control may be utilized to achieve a desired hormone level and/or mix.

#### IMPLANTATION METHOD

[0203] The implantation of controller 102 can include implantation of electrodes and implantation of the controller itself. Optionally, the two implantations are performed as a single procedure. However, it is noted that each implantation has its own characteristics. Implanting a small casing into the stomach is a well-known technique and may be performed, for example using a laproscope, using open surgery or using keyhole surgery.

[0204] Implantation of electrodes in the pancreas is not a standard procedure. Optionally, elongate, uncoiling or unfolding electrodes are used so that electrode implantation is simplified.

[0205] In an exemplary embodiment of the invention, the electrodes are implanted using a laproscopic or endoscopic procedure. Optionally, also controller 102 is inserted using a laproscope or endoscope. In an exemplary embodiment of the invention, the geometry of controller 102 is that of a cylinder, so it better passes through an endoscope (flexible, relatively narrow diameter tube) or a laproscope (rigid, relatively large diameter tube). Alternatively, controller 102 is implanted separately from the electrodes. In one example, the electrodes are implanted with a connection part (e.g., wire ends) of the electrodes easily available. A second entry wound is made and the controller is attached to the connection parts. Possibly, the electrodes are implanted connection part first. Alternatively, after the electrodes are implanted, the endoscope is retracted, leaving the connection part in the body.

[0206] Figs. 6A and 6B are flowcharts of implantation methods, in accordance with exemplary embodiments of the invention.

[0207] Fig. 6A is a flowchart 400 of a bile duct approach. First, an endoscope is brought to a bile duct, for

example through the stomach (402). The endoscope then enters the bile duct (404) for example using methods known in the art. As shown, the endoscope may travel through the bile ducts along the pancreas. Alternatively, the electrodes may be provided by a catheterization of the splenic artery or vein. Alternatively, the portal vein may be catheterized, for example via a laproscopic opening in the abdomen. The electrodes are implanted in, or alongside, the pancreas, for example in the blood vessels or the bile ducts, the pancreas being an elongated gland (406). In an exemplary embodiment of the invention, the endoscope (or an extension thereof) is first advanced to the far end of the pancreas, the electrodes are attached to the pancreas and then the endoscope is retracted, leaving the electrodes behind. Alternatively, the electrodes may be advanced out of the pancreas, by themselves or using a relative rigid and/or navigable jacket. Optionally, but not necessarily, imaging techniques, such as light, ultrasound or x-ray imaging, are used to track the electrode and/or the endoscope. The imaging may be from outside the body or from inside the body, for example from the tip of the endoscope.

[0208] Any damage to body structures is optionally repaired during endoscope/catheter retraction (408). Alternatively, other arterial and/or venous techniques may be used. In some techniques, controller 102 is implanted and then the electrodes are guided along or inside a blood vessel or other body structure to the pancreas.

[0209] In bile duct implantation, a special coating may be provided on the electrode or leads, to protect against the bile fluids. The contact part of the electrode may be embedded in tissue to prevent bile fluid damage thereto.

[0210] Fig. 6B is a flowchart 420 of an alternative implantation method. An endoscope is advanced to the duodenum or other part of the intestines adjacent the pancreas (422). Electrodes are extended from the intestines into the pancreas (424), while controller 102 remains in the intestines. The electrodes may also extend part way along the inside of the intestines. Electrodes on the far side of the pancreas may be implanted from a different part of the intestines or they pass through the pancreas. Alternatively, also the controller is pushed out through a hole formed in the side of the intestines. Alternatively, the controller is enclosed in a pocket of the intestines, the pocket optionally formed by suturing or clipping together part of the intestines. Alternatively, the controller is attached to the intestines, for example using clips or using sutures. Any damage to the intestines may then be repaired (426).

[0211] As noted above with reference to Fig. 1, controller 102 may be a wireless device, with the control circuitry separate from the electrodes. The electrodes can have individual power sources or they may be powered (or recharged) using beamed power.

[0212] In an alternative embodiment, controller 102 is a multi part device, for example comprising a plurality of mini-controllers, each mini controller controlling a differ-

ent part of the pancreas. The activities of the mini-controllers may be synchronized by communication between the controllers or by a master controller, for example in the separate, possibly external unit 116. Unit 116 may directly synchronize the mini controllers and/or may provide programming to cause them to act in a synchronized manner. An exemplary geometry for a mini-controller is that of two balls connected by a wire. Each ball is an electrode, one ball contains a power source and the other ball contains control circuitry. Communication between the mini controllers may be, for example using radio waves, optionally low frequency, or using ultrasound. Suitable transmitter and/or receiver elements (not shown) are optionally provided in the mini-controllers.

[0213] Alternatively to an implanted controller, the controller may be external to the body with the electrodes being inserted percutaneously to the pancreas, or even remaining on the out side of the body. Alternatively, the controller and the electrodes may be completely enclosed by the intestines. These "implantation" methods are sometimes preferred for temporary use of the device.

[0214] In some cases, proper implantation of sensors may be problematic, for example sensors that impale single beta cells or islets. In an optional procedure, part of the pancreas is removed, sensors and/or electrodes are attached thereto and then the removed part is inserted back into the body.

[0215] In the above embodiments, it was suggested to impale the pancreas using electrodes or electrode guides. In an exemplary embodiment of the invention, when impaling, care is taken to avoid major nerves and blood vessels. In an exemplary embodiment of the invention, the implantation of electrodes takes into account other nearby excitable tissue and avoids inadvertent stimulation of such tissue.

## CALIBRATION AND PROGRAMMING

[0216] Pancreatic controller 102 may be implanted not only, after a stable disease state is known, but also during an ongoing disease progression. Under these conditions and even in the steady state, cells that are to be controlled by controller 102 are expected to be diseased and/or over-stressed and may behave somewhat unpredictably. Thus, in an exemplary embodiment of the invention, optimizing the control of the pancreas may require calibrating the controller after it is implanted. However, it is noted that such calibration is not an essential feature of the invention and may even be superfluous, especially if a reasonable estimate of the pancreatic physiological state can be determined before implantation.

[0217] Fig. 7 is a flowchart 500 of an exemplary method of controller implantation and programming, in accordance with an exemplary embodiment of the invention. Other methods may also be practiced.

[0218] Before implantation, a patient is optionally diagnosed (502) and an expected benefit of implantation is optionally determined. It is noted however, that controller 102 may also be used for diagnostic purposes, due to its ability to take measurements over extended periods of time and determining the response of the pancreas cells to different stimuli and situations.

[0219] A controller is then implanted, for example as described above, and an initial programming provided (504). The initial programming may be performed while the controller is outside the body. However, in an exemplary embodiment of the invention, the controller is capable of extensive programming when inside the body, for example as described below, to enable the controller to selectively apply one or more of the many different logic schemes and pulses, possibly differently to one or more of the controlled areas.

[0220] During an information acquisition step (506) the behavior of the pancreas is tracked, possibly without any active control of the pancreas. This information acquisition optionally continues all through the life of the controller. In an exemplary embodiment of the invention, the acquired information is periodically- and/or continuously- reported to a treating physician, for example using external unit 116. An exemplary report is the glucose levels in the body and the main events that affected the glucose level.

[0221] Alternatively to mere information gathering, the information acquisition also uses test control sequences to determine the pancreatic response to various pulse forms and sequences.

[0222] In an exemplary embodiment of the invention, the information acquisition step is used to determine physiological pathologies and especially to detect and feedback- and/or feed-forward- mechanisms that are impaired. Such mechanisms are optionally supplemented, replaced and/or overridden by controller 102.

[0223] Alternatively or additionally, the information acquisition is geared to detecting feedback and feed-forward interactions in the pancreas, especially interactions between hormones, possibly dependent on glucose levels, hormone levels and/or stimulation history. This information may be used to provide parameters for a predetermined model of the pancreas. Alternatively, a new model may be generated, for example using a neural-network program.

[0224] Possibly, various protocols are tried on small control regions to determine their effect.

[0225] The information acquisition, and later the calibration and programming may be performed on a per-person basis or even on a per-islet or per pancreatic portion basis. Optionally, a base line programming is determined from other patients with similar disorders.

[0226] Optionally, various test sequences are timed to match patient activities such as eating, sleeping, exercising and insulin uptake. Also the programming of the controller may be adapted to a sleep schedule, meal taking schedule or other known daily, weekly or otherwise

periodic activities.

[0227] Possibly, the acquisition is enhanced with testing of hormonal levels and/or other physiological parameters for which sensors may or may not be provided on the pancreatic controller. These measurements may be used to learn which glucose levels (or other physiological parameter) and/or level changes are caused by which hormonal level. Thus, normal and/or abnormal hormonal levels can be later determined without a dedicated sensor.

[0228] Possibly the additional sensors are off-line, e.g., laboratory blood testing. Alternatively or additionally, an ambulatory monitor is provided to the patient, into which the patient enters various information.

[0229] After a better picture of how the pancreas is acting is formed, a first reprogramming (508) may be performed. Such reprogramming may use any means known in the art such as magnetic fields and electromagnetic waves. The reprogramming optionally implements partial control of the pancreas (510). Such partial control may be used to avoid overstressing the entire pancreas. Some of the controlled parts may be suppressed, for example using hyper-polarizing pulses as described above. It is noted however, that since the pancreatic damage does not usually cause immediate life threatening situations and because the pancreas is formed of a plurality of substantially independent portions, there is considerably more leeway in testing the effect of control sequences and even the long term effects of such sequences, that there is in other organs such as the heart.

[0230] In an optional step 512, the interaction of pharmaceutical or hormonal treatment with the controller may be determined. In this context it is noted that cardiac and nerve electro-physiological pharmaceuticals may be useful also for treatment of pancreatic disorders. Alternatively, pancreatic control may be desirable to offset negative side effects of such pharmaceuticals taken for non-metabolic disorders. Alternatively or additionally, the effect of pharmaceuticals on pancreatic cell behavior and/or feedback interactions, is determined.

[0231] Steps 508-512 may be repeated a plurality of times before settling down to a final programming 514. It is noted that even such final programming may be periodically reassessed (516) and then modified (518), for example, as the pancreas and/or the rest of the patient improves or degrades, or to apply various long-term effect control sequences.

[0232] In an exemplary embodiment of the invention, a tissue viability testing of the controlled and/or uncontrolled parts of the pancreas is optionally performed periodically, for example to assess patient state, to update the patient base line and to assess the efficiency of the therapy. Exemplary methods of viability testing include analyzing electrical activity, responses to changes in glucose level or insulin levels and/or responses to various types of electrical stimulation.

[0233] In an exemplary embodiment of the invention,

the programming, measurements and/or prior attempted treatments (including possibly pharmaceutical treatments) are stored in a memory portion of controller 102. Alternatively or additionally, the programming may include special sequences that take into account taking of pharmaceuticals. In an exemplary embodiment of the invention, when a patient takes a pharmaceutical or insulin controller 102 is notified, for example by manual input into external unit 116 or automatically by the administration method. If the patient neglected to take the pharmaceutical, insulin, and/or glucose, a compensatory control sequence is provided, possibly irrespective of whether an alert is provided to the patient.

#### EXPERIMENT

[0234] In an exemplary experiment, a mesh unipolar electrode was placed under a pig pancreas and a needle electrode was inserted into the overlying abdominal wall as a ground. A pulsed current (5 Hz, 5 mA, 5 ms duration) was applied for five minutes and resulted in decrease in serum glucose from 89 to 74 mg/dl. Serum insulin increased from 3.8 to 5.37, microU/ml, measured using the ELISA method. Both glucose levels and insulin levels returned to the baseline after 30 minutes. In a different animal, the application for 5 minutes of a pulse of 3 Hz, 12 mA and 5 ms duration resulted in an insulin increase from 8.74 microU/ml to 10.85 8.74 microU/ml. [0235] Fig. 8 is a chart showing the effect of such electrical stimulation on insulin levels, in six animals.

#### ADDITIONAL EXPERIMENTS

[0236] Fig. 9 is a chart showing the effect of electrical stimulation on blood glucose levels, in an experiment in which glucose levels are increased faster than would be expected solely by inhibition of insulin secretion.

[0237] In a sub-chart 904 of chart 900, glucose levels are reduced by the application of a stimulation pulse S1. In a sub-chart 902 of chart 900, glucose levels are increased by the application of a stimulation pulse S2 and then reduced by an application of pulse S1 again. It is hypothesized that merely reducing insulin secretion would not be sufficient to explain such a fast and large increase in glucose levels. Instead, the secretion of glucagon is causing a release of glucose from the liver, raising the blood glucose level.

[0238] Chart 900 is from an experiment on a rat which was anesthetized with pentobarbitine (40 mg/1 Kg). After fasting the rat was given a continuous infusion of 5% glucose at a rate of 2 cc/Hr. During the experiment, the rat was ventilated with oxygen. The sample shown on chart 900 are the results of an analysis by a glucometer "Glucotrend", by Rosche, of blood from the right jugular vein every 5 minutes. S1 and S2 have a similar form, except that S2 has a 2mA amplitude and a 3.5 minute duration, while S1 has a 1mA amplitude and a 5 minute duration. The pulse includes an initial spike followed by

a 150 ms delay and a train of 7 50% duty cycle spikes spread over 400 ms. The entire pulse is repeated every 10 seconds. The initial spike is 50 ms long. Both electrodes were Iridium Oxide coated Titanium. The geometry of the electrodes was a coil, 8 mm long, 1.2 mm diameter, with a 100  $\mu$  diameter 3 filler wire. The coil was glued on a silicone pad (for insulation and prevention of mechanical damage). Two such electrodes were placed along the pancreas, one above and one below (when the rat is on its back).

[0239] Figs. 10A-10B, 11A-11B, 12A-12B and 13A-13B are pairs of figures, each pair showing a chart and a pulse diagram of an additional experiments using a similar setup to that of Fig. 9.

[0240] In Figs. 10, 12 and 13 both electrodes were above the pancreas and the signal was applied for 5 minutes.

[0241] In Fig. 11, both electrodes were under the pancreas and the signal was applied for 5 minutes.

#### EXEMPLARY APPLICATIONS

[0242] The above pancreatic controller 102 may be used after a diabetic state is identified. Optionally however, the controller is used to better diagnose an evolving disease state and/or to prevent a final diabetic state from ever occurring, for example by supporting the pancreas. Thus, a temporary device embodiment is optionally provided additionally to permanently implanted device.

[0243] In another application, strict control of body insulin output and blood glucose levels is used not only to prevent obese patient from developing diabetes by overworking of the pancreas, but also (simultaneously or alternatively) for reducing body weight. Such a scheme may require strict prevention of elevated glucose levels in blood, to avoid damage to the body. However, it is expected that by reducing insulin production at "normal" glucose levels, feelings of hunger may be suppressed, as well as reducing the increase in mass of adipose tissue.

[0244] In an exemplary embodiment of the invention, controller 102 is a stand alone device. However, a dual organ controller may be useful in some disease states. In one example, it is noted that many patients with pancreatic disorders also have cardiac problems. Thus, a combined cardiac/pancreatic controller may be provided, possibly sharing one or more of a casing, programming means, power supply and control circuitry. In another example, a controller for the uterus and a pancreatic controller may be combined to protect against pregnancy related diabetes and improper uterine contractions.

[0245] Another exemplary dual organ controller is used for both the stomach and the pancreas. Such a controller is useful for obese persons, to suppress stomach contractions and prevent feelings of hunger. At the same time, insulin level may be controlled to prevent

hunger, or, in diabetic patients, to prevent hyper- or hypo- glycemia.

[0246] Also within the scope of the invention are surgical kits which include sets of medical devices suitable for implanting a controller and such a controller. Section headers are provided only to assist in navigating the application and should not be construed as necessarily limiting the contents described in a certain section, to that section. Measurements are provided to serve only as exemplary measurements for particular cases, the exact measurements applied will vary depending on the application. When used in the following claims, the terms "comprises", "comprising", "includes", "including" or the like means "including but not limited to".

[0247] It will be appreciated by a person skilled in the art that the present invention is not limited by what has thus far been described. Rather, the scope of the present invention is limited only by the following claims.

#### Claims

1. A pancreatic controller, comprising:

at least one electrode (112) adapted for electrifying at least a portion of a pancreas (100); and a controller (102) programmed to electrify said at least one electrode (112),

#### characterized in that:

said controller (102) is adapted to control at least two members of a group consisting of blood glucose level, blood insulin level and blood level of another pancreatic hormone, in a manner incompatible with a causative interaction between the at least two members.

2. A controller according to claim 1, wherein said controller (102) is adapted to modify said at least two members simultaneously.
3. A controller according to claim 1, wherein said controller (102) is adapted to selectively modify only one of said at least two members, while at least reducing a causative interaction between said two members.
4. A controller according to any of claims 1-3, wherein said controller (102) is adapted to maintain at least one of said members within a desired physiologic range.
5. A controller according to any of claims 1-4, wherein said at least two members comprise glucose level and insulin level.
6. A controller according to claim 5, wherein said con-

troller (102) is adapted to modulate an effect of said insulin not related to carbohydrate metabolism.

7. A controller according to any of claims 1-6, wherein at least one of said two members comprise glucagon.
8. A controller according to claim 7, wherein said controller (102) is adapted to increase glucagon secretion, to counteract an effect of insulin
9. A controller according to claim 7 or claim 8, wherein said controller (102) is adapted to increase glucagon secretion, to achieve higher blood glucose levels.
10. A controller according to claim 7, wherein said controller (102) is adapted to reduce the secretion of glucagon, when insulin secretion is increased.
11. A controller according to any of claims 1-10, wherein at least one of said two members comprise Somatostatin.
12. A controller according to any of claims 1-11, wherein at least one of said members comprises glucose level.
13. A controller according to claim 12, wherein said controller (102) is adapted to select between alternative control therapies, a therapy that has a least disrupting effect on said glucose levels.
14. A controller according to any of claims 1-13, wherein said controller (102) uses solely electrical fields to control said members.
15. A controller according to any of claims 1-13, wherein said controller (102) is adapted to take molecules provided in the body, into account, for said control.
16. A controller according to claim 15, wherein said controller (102) does not control the provision of said molecules.
17. A controller according to claim 15, wherein said controller (102) is adapted to control the provision of said molecules.
18. A controller according to any of claims 15-17, wherein said molecules suppress the secretion of at least one pancreatic hormone.
19. A controller according to any of claims 15-17, wherein said molecules suppress the effect of at least one pancreatic hormone.
20. A controller according to any of claims 15-17,

wherein said molecules enhance the secretion of at least one pancreatic hormone.

21. A controller according to any of claims 15-17, wherein said molecules enhance the effect of at least one pancreatic hormone.

22. A controller according to any of claims 1-21, wherein said controller (102) is adapted to suppress a secretion of an antagonistic hormone.

23. A controller according to any of claims 1-22, wherein said controller (102) is adapted to enhance a secretion of an antagonistic hormone.

24. A controller according to any of claims 1-21, wherein said controller (102) is adapted to store therein feedback interactions of said pancreas.

25. A controller according to claim 24, wherein said feedback interactions comprise interactions between hormone levels.

26. A controller according to any of claims 24-25, wherein said feedback interactions are dependent on blood glucose levels.

27. A controller according to any of claims 24-26, wherein said controller (102) is adapted to determine said feedback interactions, by tracking a behavior of said pancreas (100).

28. A controller according to claim 27, wherein said controller (102) is adapted to actively modify at least one of a glucose level and a pancreatic hormone level, to collect feedback interaction information.

29. A controller according to any of claims 1-28, comprising one or more sensors (114, 118) for sensing a level of said controlled member.

30. A controller according to any of claims 1-29, wherein said controller (102) is adapted to estimate a level of said controlled member.

31. A controller according to any of claims 1-30, wherein said controller (102) is adapted to electrify said electrode (112) to apply a non-excitatory pulse to effect said control.

32. A controller according to any of claims 1-30, wherein said controller (102) is adapted to electrify said electrode (112) to apply an excitatory pulse to effect said control.

33. A controller according to any of claims 1-30, wherein said controller (102) is adapted to electrify said electrode (112) to modify blood flow associated with

said pancreas (100) to effect said control.

34. A controller according to claim 33, wherein said modified blood flow comprises blood flow to hormone generating cells of said pancreas.

35. A controller according to claim 33, wherein said modified blood flow comprises blood flow from said pancreas (100).

36. A controller according to claim 33, wherein said modified blood flow comprises blood flow from hormone generating cells of said pancreas.

37. A controller according to any of claims 1-36, wherein said at least one electrode (112) comprises at least two electrodes for placement in different regions of said pancreas (100); and wherein said controller (102) is adapted to selectively electrify different regions of said pancreas (100), to achieve a desired control by said at least two members.

38. A controller according to any of claims 1-37, wherein said controller (102) is adapted to control secretion.

39. A controller according to any of claims 1-38, wherein said controller (102) is adapted to control production.

40. A controller according to any of claims 1-38, wherein said controller (102) is adapted to control physiological activity.

#### Patentansprüche

1. Pankreassteuervorrichtung, umfassend:

mindestens eine Elektrode (112), die angepasst ist, um mindestens einen Teil eines Pankreas (100) zu elektrisieren; und eine Steuervorrichtung (102), die programmiert ist, um die mindestens eine Elektrode (112) zu elektrisieren, **dadurch**

**gekennzeichnet, dass:**

die Steuervorrichtung (102) angepasst ist, um mindestens zwei Elemente einer Gruppe, die aus Blutglukosespiegel, Blutinsulinspiegel und Blutspiegel eines anderen Pankreashormons zusammengesetzt ist, auf eine Weise zu steuern, die mit einer kausativen Wechselwirkung zwischen den mindestens zwei Elementen unvereinbar ist.

2. Steuervorrichtung nach Anspruch 1, wobei die Steuervorrichtung (102) angepasst ist, um die mindestens zwei Elemente gleichzeitig zu modifizieren.
3. Steuervorrichtung nach Anspruch 1, wobei die Steuervorrichtung (102) angepasst ist, um nur eines von den mindestens zwei Elementen selektiv zu modifizieren, während mindestens eine kausative Wechselwirkung zwischen den zwei Elementen verringert wird.
4. Steuervorrichtung nach einem der Ansprüche 1-3, wobei die Steuervorrichtung (102) angepasst ist, um mindestens eines von den Elementen in einem gewünschten physiologischen Bereich zu halten.
5. Steuervorrichtung nach einem der Ansprüche 1-4, bei der die mindestens zwei Elemente Glukosespiegel und Insulinspiegel umfassen.
6. Steuervorrichtung nach Anspruch 5, wobei die Steuervorrichtung (102) angepasst ist, um eine Wirkung des Insulins zu modulieren, die nicht mit dem Kohlehydratstoffwechsel in Beziehung steht.
7. Steuervorrichtung nach einem der Ansprüche 1-6, bei der mindestens eines der zwei Elemente Glucagon umfasst.
8. Steuervorrichtung nach Anspruch 7, wobei die Steuervorrichtung (102) angepasst ist, um eine Glucagonsekretion zu erhöhen, um einer Wirkung von Insulin entgegenzuwirken.
9. Steuervorrichtung nach Anspruch 7 oder Anspruch 8, wobei die Steuervorrichtung (102) angepasst ist, um eine Glucagonsekretion zu erhöhen, um höhere Blutglukosespiegel zu erzielen.
10. Steuervorrichtung nach Anspruch 7, wobei die Steuervorrichtung (102) angepasst ist, um die Sekretion von Glucagon zu verringern, wenn eine Insulinsekretion erhöht ist.
11. Steuervorrichtung nach einem der Ansprüche 1-10, bei der mindestens eines der zwei Elemente Somatostatin umfasst.
12. Steuervorrichtung nach einem der Ansprüche 1-11, bei der mindestens eines der Elemente einen Glukosespiegel umfasst.
13. Steuervorrichtung nach Anspruch 12, wobei die Steuervorrichtung (102) angepasst ist, um unter alternativen Steuertherapien eine Therapie auszuwählen, die mindestens eine unterbrechende Wirkung auf die Glukosespiegel aufweist.
14. Steuervorrichtung nach einem der Ansprüche 1-13, wobei die Steuervorrichtung (102) lediglich elektrische Felder verwendet, um die Elemente zu steuern.
15. Steuervorrichtung nach einem der Ansprüche 1-13, wobei die Steuervorrichtung (102) angepasst ist, um Moleküle, die im Körper bereitgestellt werden, für die Steuerung zu berücksichtigen.
16. Steuervorrichtung nach Anspruch 15, wobei die Steuervorrichtung (102) die Bereitstellung der Moleküle nicht steuert.
17. Steuervorrichtung nach Anspruch 15, wobei die Steuervorrichtung (102) angepasst ist, um die Bereitstellung der Moleküle zu steuern.
18. Steuervorrichtung nach einem der Ansprüche 15-17, bei der die Moleküle die Sekretion von mindestens einem Pankreashormon unterdrücken.
19. Steuervorrichtung nach einem der Ansprüche 15-17, bei der die Moleküle die Wirkung von mindestens einem Pankreashormon unterdrücken.
20. Steuervorrichtung nach einem der Ansprüche 15-17, bei der die Moleküle die Sekretion von mindestens einem Pankreashormon steigern.
21. Steuervorrichtung nach einem der Ansprüche 15-17, bei der die Moleküle die Wirkung von mindestens einem Pankreashormon steigern.
22. Steuervorrichtung nach einem der Ansprüche 1-21, wobei die Steuervorrichtung (102) angepasst ist, um eine Sekretion eines antagonistischen Hormons zu unterdrücken.
23. Steuervorrichtung nach einem der Ansprüche 1-22, wobei die Steuervorrichtung (102) angepasst ist, um eine Sekretion eines antagonistischen Hormons zu steigern.
24. Steuervorrichtung nach einem der Ansprüche 1-21, wobei die Steuervorrichtung (102) angepasst ist, um darin Rückkopplungswechselwirkungen des Pankreas zu speichern.
25. Steuervorrichtung nach Anspruch 24, bei der die Rückkopplungswechselwirkungen Wechselwirkungen zwischen Hormonspiegeln umfassen.
26. Steuervorrichtung nach einem der Ansprüche 24-25, bei der die Rückkopplungswechselwirkungen vom Blutglukosespiegel abhängen.
27. Steuervorrichtung nach einem der Ansprüche

24-26, wobei die Steuervorrichtung (102) angepasst ist, um die Rückkopplungswechselwirkungen durch Verfolgen eines Verhaltens des Pankreas (100) zu bestimmen.

28. Steuervorrichtung nach Anspruch 27, wobei die Steuervorrichtung (102) angepasst ist, um mindestens einen von einem Glukosespiegel und einem Pankreashormonspiegel aktiv zu modifizieren, um eine Rückkopplungswechselwirkungsinformation zu sammeln.
29. Steuervorrichtung nach einem der Ansprüche 1-28, umfassend einen oder mehrere Sensoren (114, 118), um einen Spiegel des gesteuerten Elements zu erfassen.
30. Steuervorrichtung nach einem der Ansprüche 1-29, wobei die Steuervorrichtung (102) angepasst ist, um einen Spiegel des gesteuerten Elements zu veranschlagen.
31. Steuervorrichtung nach einem der Ansprüche 1-30, wobei die Steuervorrichtung (102) angepasst ist, um die Elektrode (112) zu elektrisieren, um einen Nicht-Erregungsimpuls anzulegen, um die Steuerung zu bewerkstelligen.
32. Steuervorrichtung nach einem der Ansprüche 1-30, wobei die Steuervorrichtung (102) angepasst ist, um die Elektrode (112) zu elektrisieren, um einen Erregungsimpuls anzulegen, um die Steuerung zu bewerkstelligen.
33. Steuervorrichtung nach einem der Ansprüche 1-30, wobei die Steuervorrichtung (102) angepasst ist, um die Elektrode (112) zu elektrisieren, um einen Blutfluss zu modifizieren, der mit dem Pankreas (100) verbunden ist, um die Steuerung zu bewerkstelligen.
34. Steuervorrichtung nach Anspruch 33, bei der der modifizierte Blutfluss einen Blutfluss zu Hormon-erzeugenden Zellen des Pankreas umfasst.
35. Steuervorrichtung nach Anspruch 33, bei der der modifizierte Blutfluss Blutfluss von dem Pankreas (100) umfasst.
36. Steuervorrichtung nach Anspruch 33, bei der der modifizierte Blutfluss Blutfluss von Hormon-erzeugenden Zellen des Pankreas umfasst.
37. Steuervorrichtung nach einem der Ansprüche 1-36, bei der die mindestens eine Elektrode (112) mindestens zwei Elektroden zur Platzierung in unterschiedlichen Gebieten des Pankreas (100) umfasst; und

wobei die Steuervorrichtung (102) angepasst ist, um unterschiedliche Gebiete des Pankreas (100) selektiv zu elektrisieren, um eine gewünschte Steuerung durch die mindestens zwei Elemente zu erzielen.

38. Steuervorrichtung nach einem der Ansprüche 1-37, wobei die Steuervorrichtung (102) angepasst ist, um eine Sekretion zu steuern.
39. Steuervorrichtung nach einem der Ansprüche 1-38, wobei die Steuervorrichtung (102) angepasst ist, um eine Produktion zu steuern.
40. Steuervorrichtung nach einem der Ansprüche 1-38, wobei die Steuervorrichtung (102) angepasst ist, um eine physiologische Aktivität zu steuern.

## Revendications

### 1. Régulateur pancréatique, comprenant :

au moins une électrode (112) adaptée pour électrifier au moins une partie d'un pancréas (100) ; et  
un régulateur (102) programmé pour électrifier ladite au moins une électrode (112),

### caractérisé en ce que :

ledit régulateur (102) est adapté pour réguler au moins deux éléments d'un groupe comprenant le niveau de glucose dans le sang, le niveau d'insuline dans le sang et le niveau dans le sang d'une autre hormone pancréatique, d'une manière incompatible avec une interaction causale entre les au moins deux éléments.

2. Régulateur selon la revendication 1, dans lequel ledit régulateur (102) est adapté pour modifier lesdits au moins deux éléments de façon simultanée.
3. Régulateur selon la revendication 1, dans lequel ledit régulateur (102) est adapté pour modifier sélectivement un seul desdits au moins deux éléments, tout en réduisant au moins une interaction causale entre lesdits deux éléments.
4. Régulateur selon l'une quelconque des revendications 1 à 3, dans lequel ledit régulateur (102) est adapté pour maintenir au moins un desdits éléments à l'intérieur d'une plage physiologique souhaitée.
5. Régulateur selon l'une quelconque des revendications 1 à 4, dans lequel lesdits au moins deux éléments comprennent un niveau de glucose et un ni-

veau d'insuline.

6. Régulateur selon la revendication 5, dans lequel ledit régulateur (102) est adapté pour moduler un effet de ladite insuline qui n'est pas lié au métabolisme des glucides. 5
7. Régulateur selon l'une quelconque des revendications 1 à 6, dans lequel au moins un desdits deux éléments comprend le glucagon. 10
8. Régulateur selon la revendication 7, dans lequel ledit régulateur (102) est adapté pour augmenter une sécrétion de glucagon, afin de neutraliser un effet de l'insuline. 15
9. Régulateur selon la revendication 7 ou la revendication 8, dans lequel ledit régulateur (102) est adapté pour augmenter la sécrétion de glucagon, afin d'obtenir des niveaux de glucose dans le sang plus élevés. 20
10. Régulateur selon la revendication 7, dans lequel ledit régulateur (102) est adapté pour réduire la sécrétion de glucagon, lorsque la sécrétion d'insuline est augmentée. 25
11. Régulateur selon l'une quelconque des revendications 1 à 10, dans lequel au moins un desdits deux éléments comprend la somatostatine. 30
12. Régulateur selon l'une quelconque des revendications 1 à 11, dans lequel au moins un desdits éléments comprend le niveau de glucose. 35
13. Régulateur selon la revendication 12, dans lequel ledit régulateur (102) est adapté pour choisir parmi des variantes de thérapies de régulation, la thérapie qui a un effet le moins perturbateur sur lesdits niveaux de glucose. 40
14. Régulateur selon l'une quelconque des revendications 1 à 13, dans lequel ledit régulateur (102) utilise uniquement des champs électriques pour réguler lesdits éléments. 45
15. Régulateur selon l'une quelconque des revendications 1 à 13, dans lequel ledit régulateur (102) est adapté pour prendre en compte des molécules présentes dans le corps pour ladite régulation. 50
16. Régulateur selon la revendication 15, dans lequel ledit régulateur (102) ne régule pas la présence desdites molécules. 55
17. Régulateur selon la revendication 15, dans lequel ledit régulateur (102) est adapté pour réguler la présence desdites molécules.
18. Régulateur selon l'une quelconque des revendications 15 à 17, dans lequel lesdites molécules suppriment la sécrétion d'au moins une hormone pancréatique.
19. Régulateur selon l'une quelconque des revendications 15 à 17, dans lequel lesdites molécules suppriment l'effet d'au moins une hormone pancréatique.
20. Régulateur selon l'une quelconque des revendications 15 à 17, dans lequel lesdites molécules augmentent la sécrétion d'au moins une hormone pancréatique.
21. Régulateur selon l'une quelconque des revendications 15 à 17, dans lequel lesdites molécules augmentent l'effet d'au moins une hormone pancréatique.
22. Régulateur selon l'une quelconque des revendications 1 à 21, dans lequel le régulateur (102) est adapté pour supprimer une sécrétion d'une hormone antagoniste.
23. Régulateur selon l'une quelconque des revendications 1 à 22, dans lequel ledit régulateur (102) est adapté pour augmenter une sécrétion d'une hormone antagoniste.
24. Régulateur selon l'une quelconque des revendications 1 à 21, dans lequel ledit régulateur (102) est adapté pour stocker les interactions de rétrocontrôle dudit pancréas.
25. Régulateur selon la revendication 24, dans lequel lesdites interactions de rétrocontrôle comprennent des interactions entre les niveaux d'hormones.
26. Régulateur selon l'une quelconque des revendications 24 et 25, dans lequel lesdites interactions de rétrocontrôle dépendent des niveaux de glucose dans le sang.
27. Régulateur selon l'une quelconque des revendications 24 à 26, dans lequel ledit régulateur (102) est adapté pour déterminer lesdites interactions de rétrocontrôle, en suivant un comportement dudit pancréas (100).
28. Régulateur selon la revendication 27, dans lequel ledit régulateur (102) est adapté pour modifier activement au moins un d'un niveau de glucose et d'un niveau d'hormone pancréatique, pour recueillir les informations d'interaction de rétrocontrôle.
29. Régulateur selon l'une quelconque des revendications 1 à 28, comprenant un ou plusieurs capteurs

- (114, 118) pour détecter un niveau dudit élément régulé.
30. Régulateur selon l'une quelconque des revendications 1 à 29, dans lequel ledit régulateur (102) est adapté pour estimer un niveau dudit élément régulé. 5
31. Régulateur selon l'une quelconque des revendications 1 à 30, dans lequel ledit régulateur (102) est adapté pour électrifier ladite électrode (112) afin d'appliquer une impulsion non-excitatrice pour effectuer ladite régulation. 10
32. Régulateur selon l'une quelconque des revendications 1 à 30, dans lequel ledit régulateur (102) est adapté pour électrifier ladite électrode (112) afin d'appliquer une impulsion excitatrice pour effectuer ladite régulation. 15
33. Régulateur selon l'une quelconque des revendications 1 à 30, dans lequel ledit régulateur (102) est adapté pour électrifier ladite électrode (112) afin de modifier le flux sanguin associé audit pancréas (100) pour effectuer ladite régulation. 20
34. Régulateur selon la revendication 33, dans lequel ledit flux sanguin modifié comprend le flux sanguin vers les cellules de génération d'hormones dudit pancréas. 25
35. Régulateur selon la revendication 33, dans lequel ledit flux sanguin modifié comprend le flux sanguin provenant dudit pancréas (100). 30
36. Régulateur selon la revendication 33, dans lequel ledit flux sanguin modifié comprend le flux sanguin provenant des cellules de génération d'hormones dudit pancréas. 35
37. Régulateur selon l'une quelconque des revendications 1 à 36, dans lequel ladite au moins une électrode (112) comprend au moins deux électrodes pour placement dans différentes régions dudit pancréas (100) ; et 40
- dans lequel ledit régulateur (102) est adapté pour identifier de façon sélective différentes régions dudit pancréas (100), afin d'obtenir une régulation souhaitée par lesdits au moins deux éléments. 45
38. Régulateur selon l'une quelconque des revendications 1 à 37, dans lequel ledit régulateur (102) est adapté pour réguler la sécrétion. 50
39. Régulateur selon l'une quelconque des revendications 1 à 38, dans lequel ledit régulateur (102) est adapté pour réguler la production. 55
40. Régulateur selon l'une quelconque des revendications 1 à 38, dans lequel ledit régulateur (102) est adapté pour réguler l'activité physiologique.

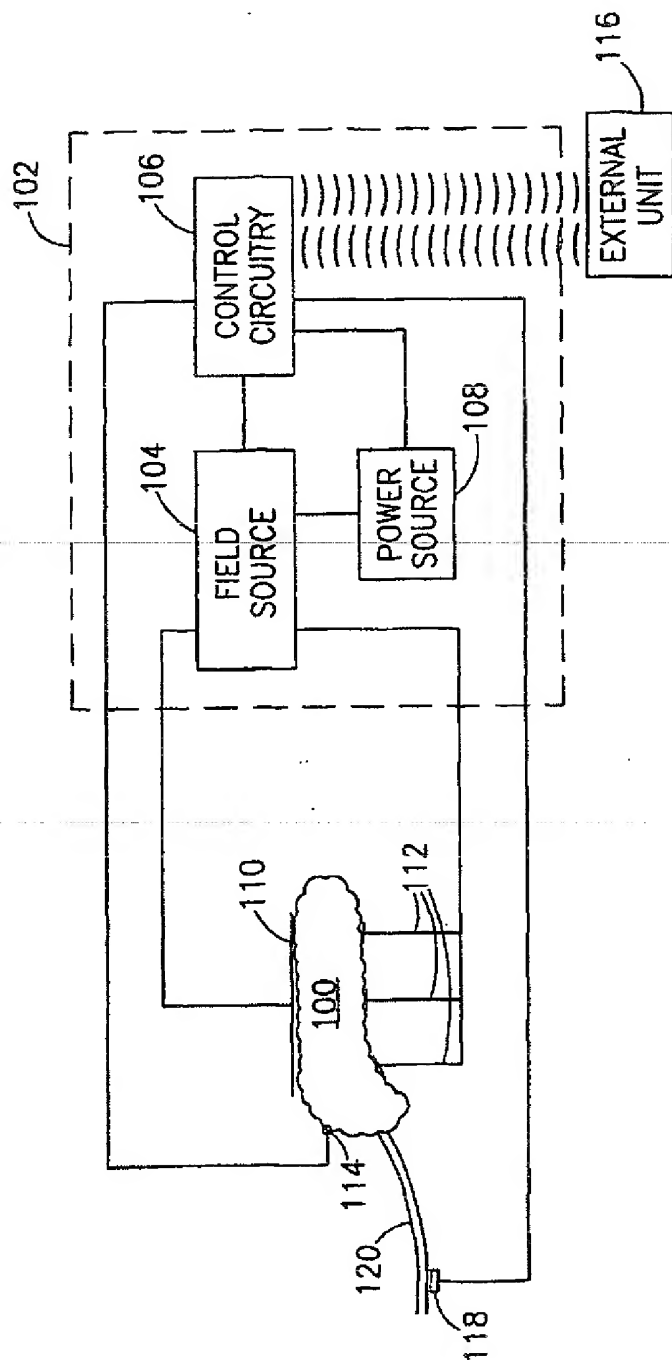


FIG.1

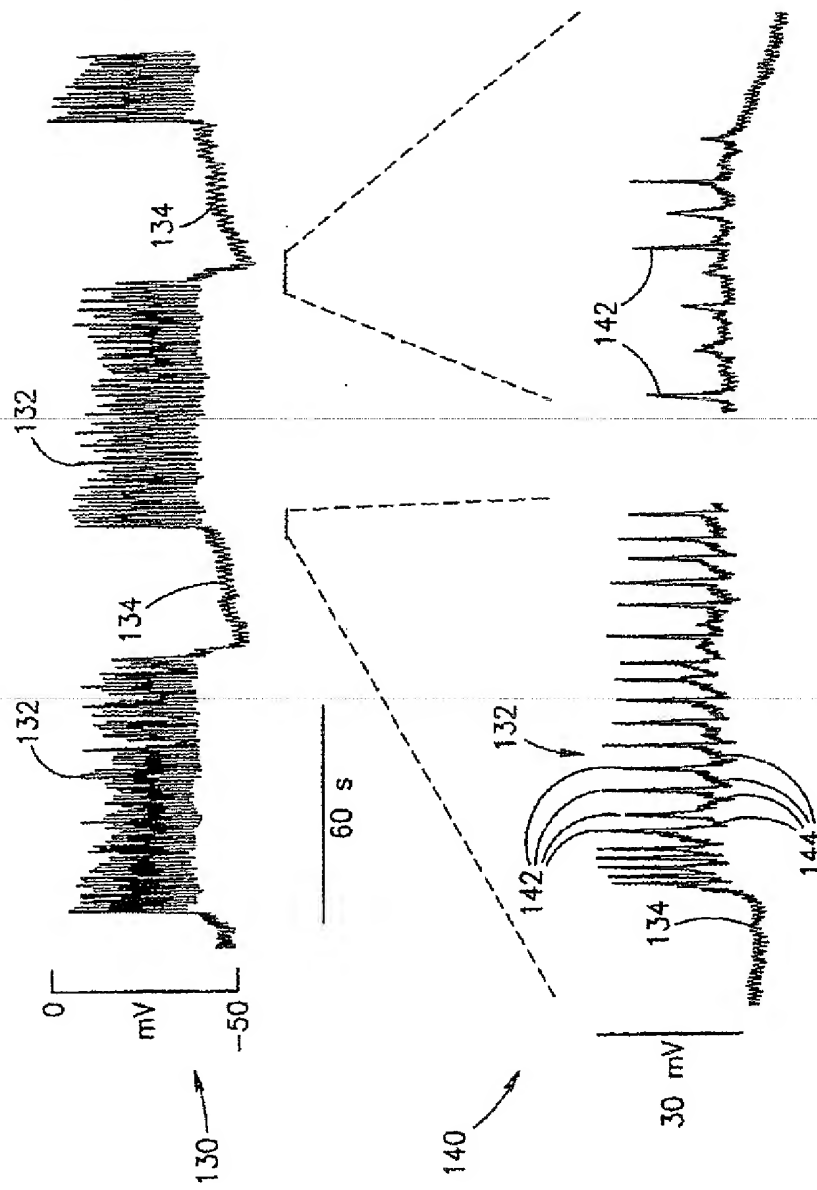


FIG.2

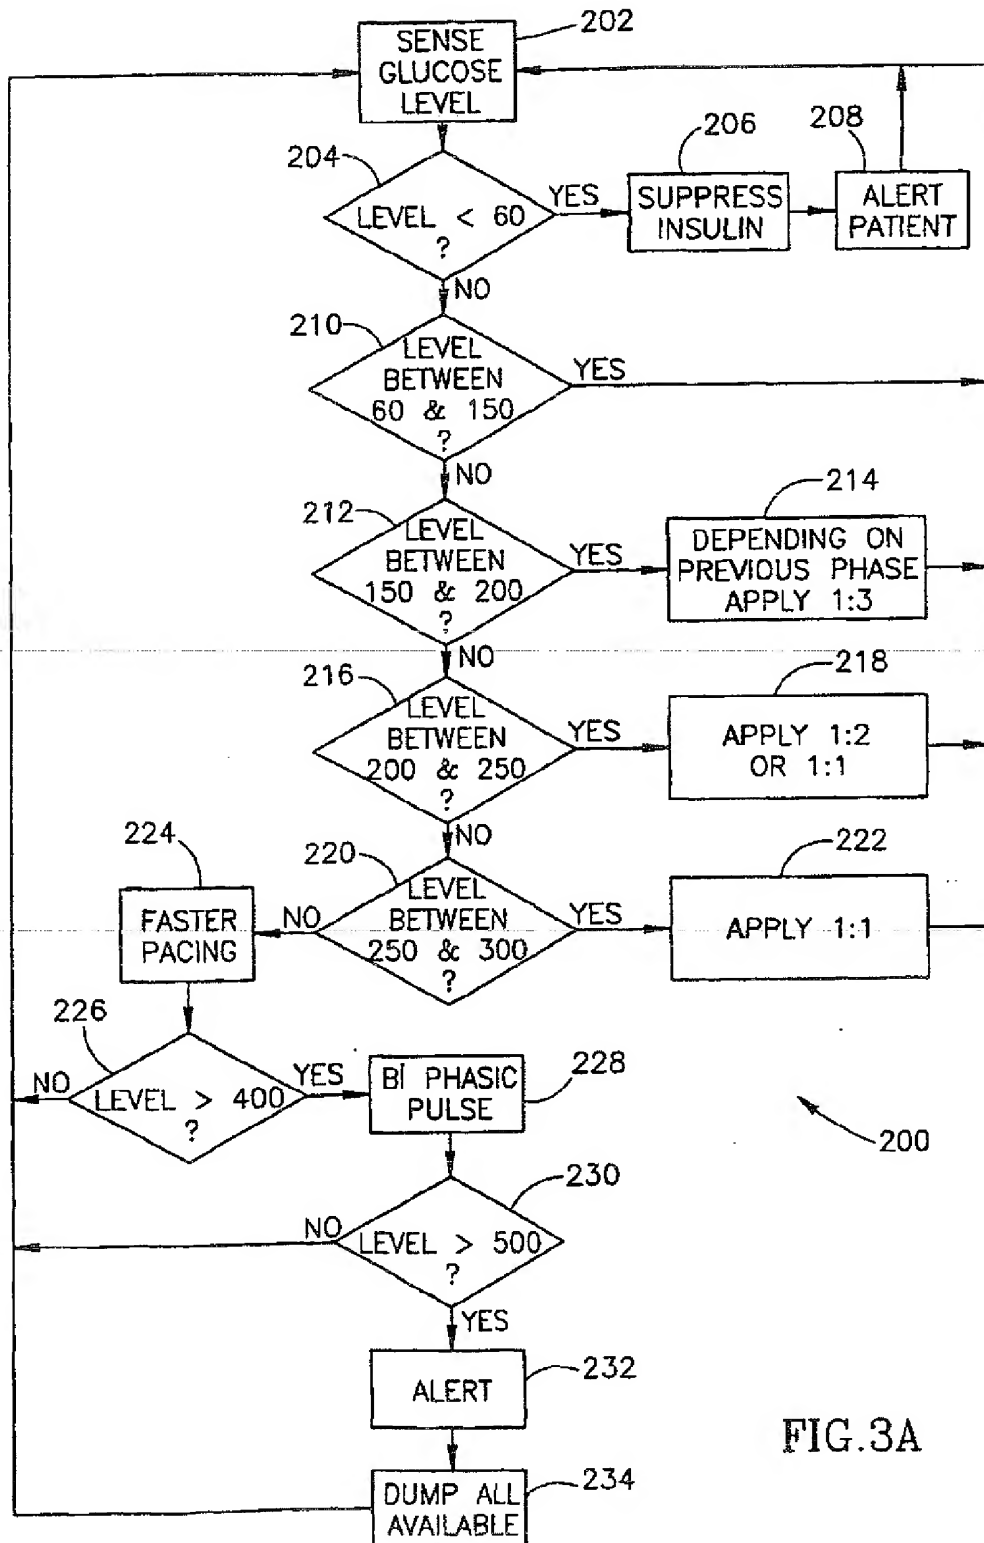


FIG. 3A

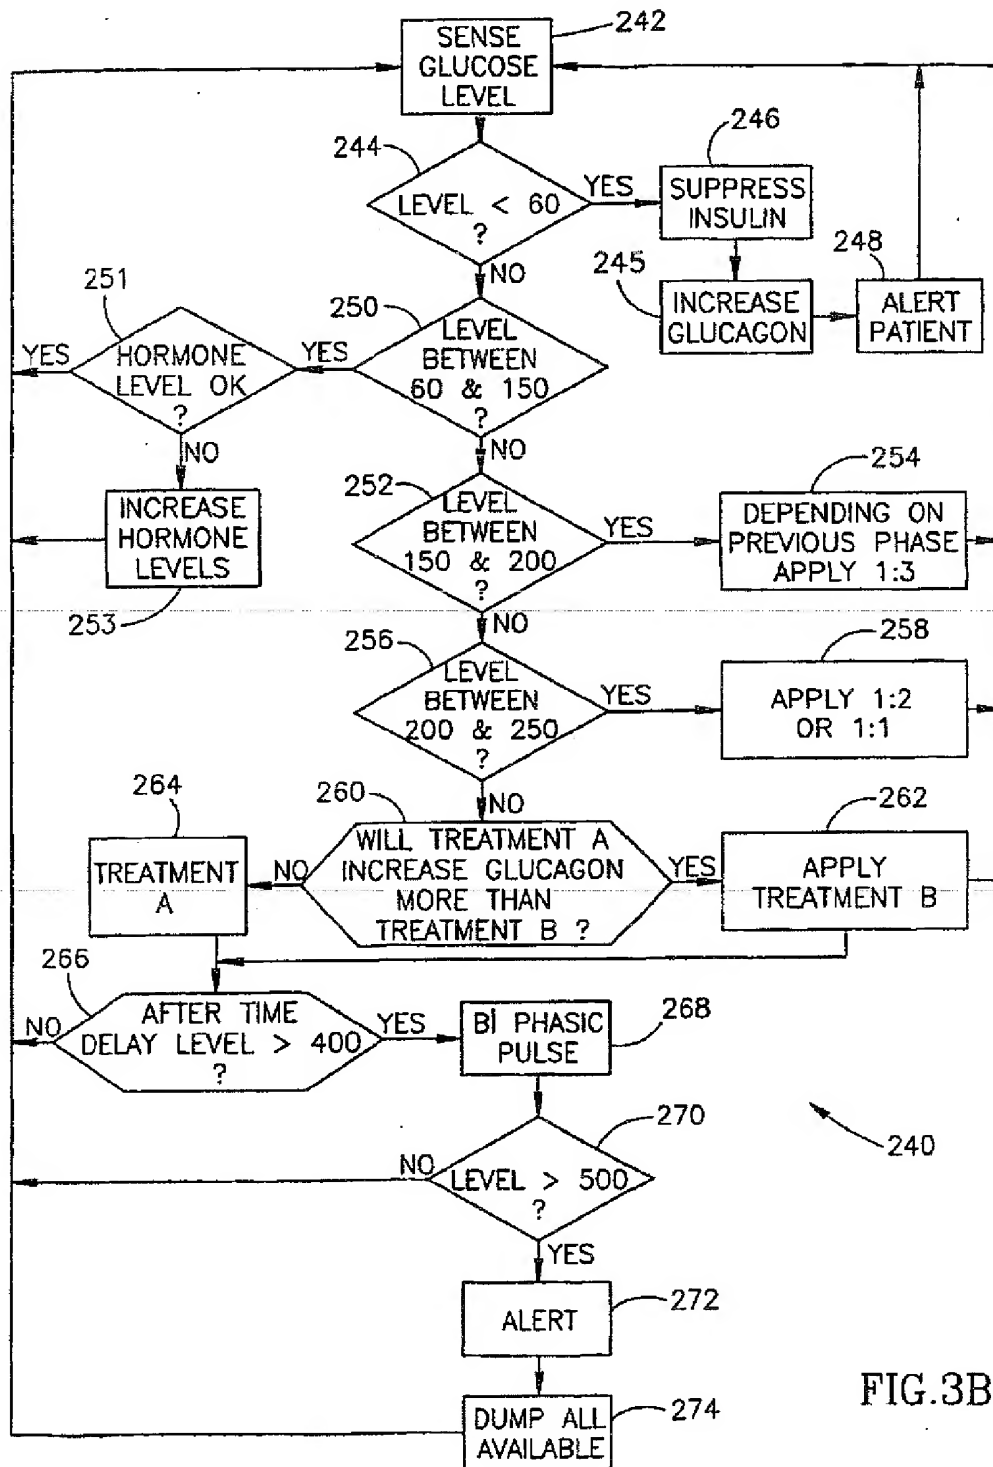


FIG.3B

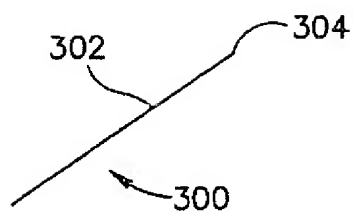


FIG. 4A

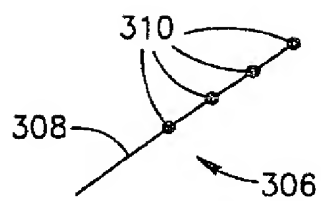


FIG. 4B

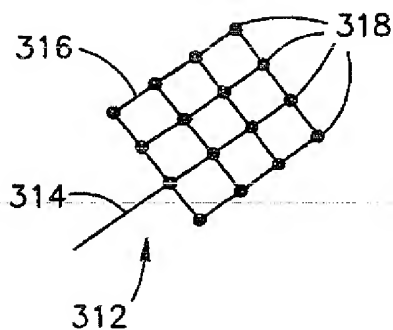


FIG. 4C

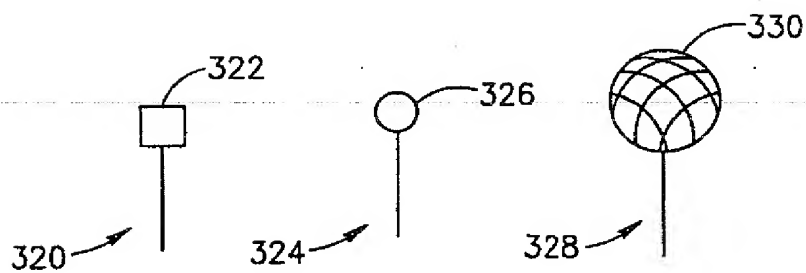


FIG. 4D

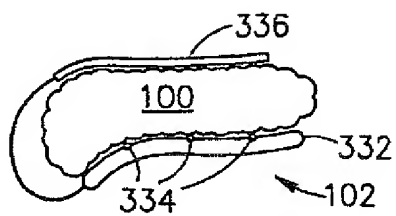


FIG. 4E



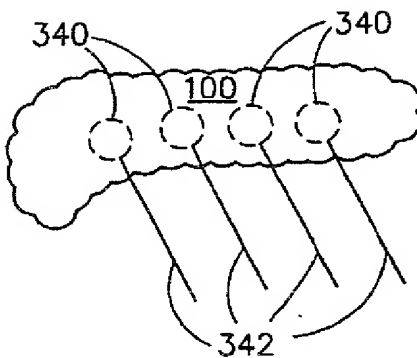


FIG. 5

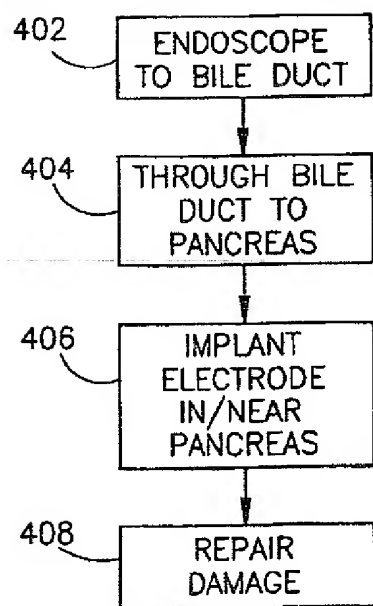

400

FIG. 6A

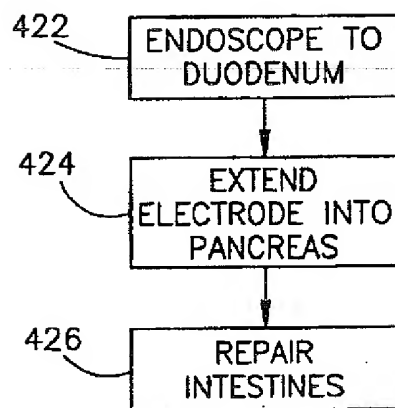

420

FIG. 6B

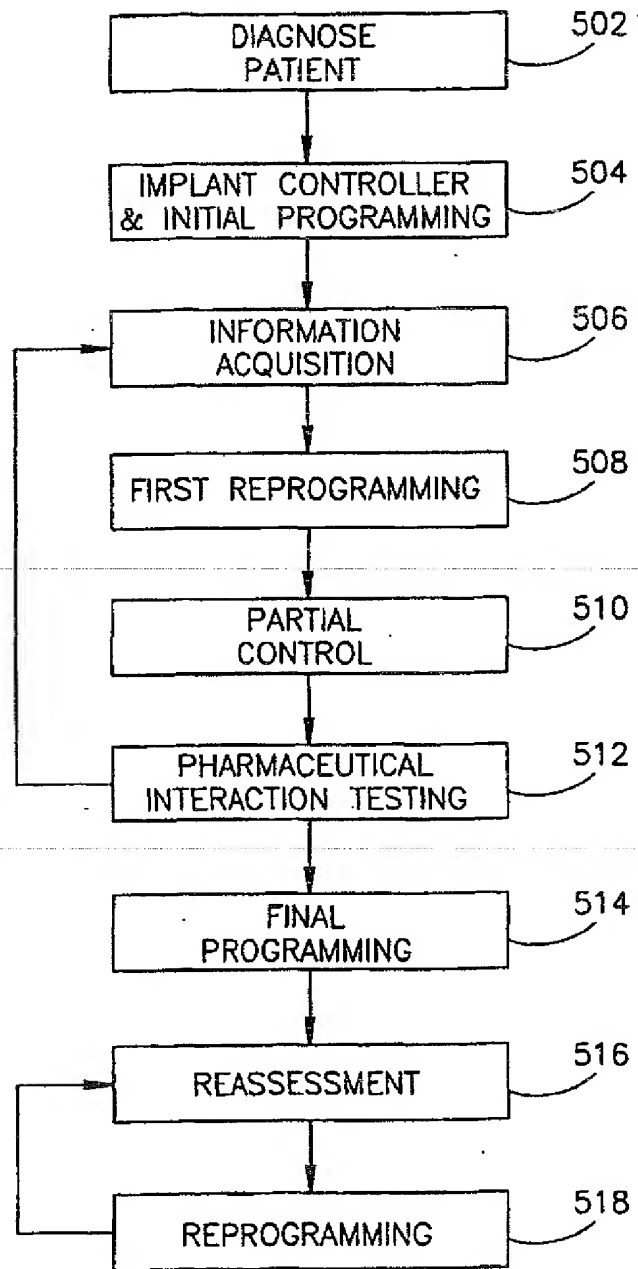


FIG.7

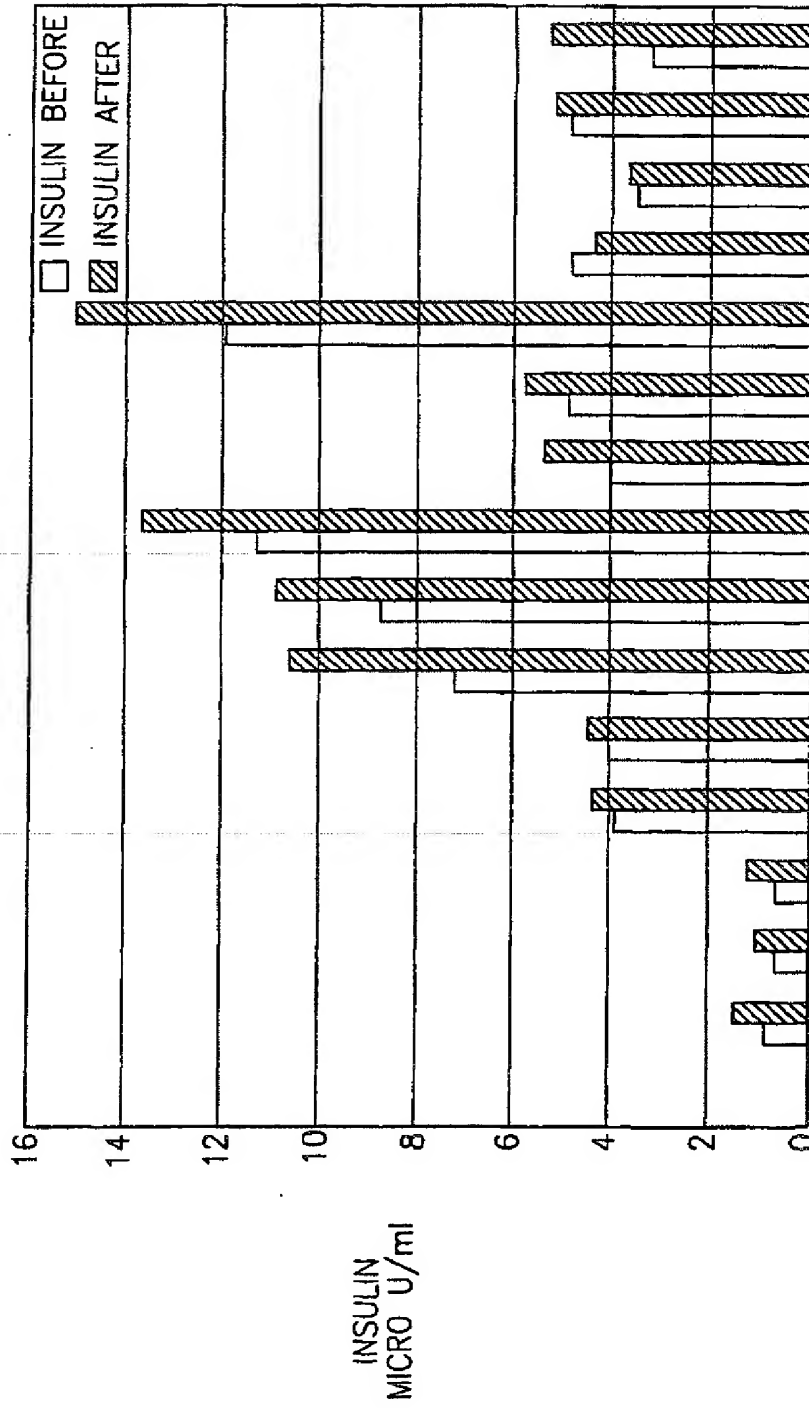


FIG.8

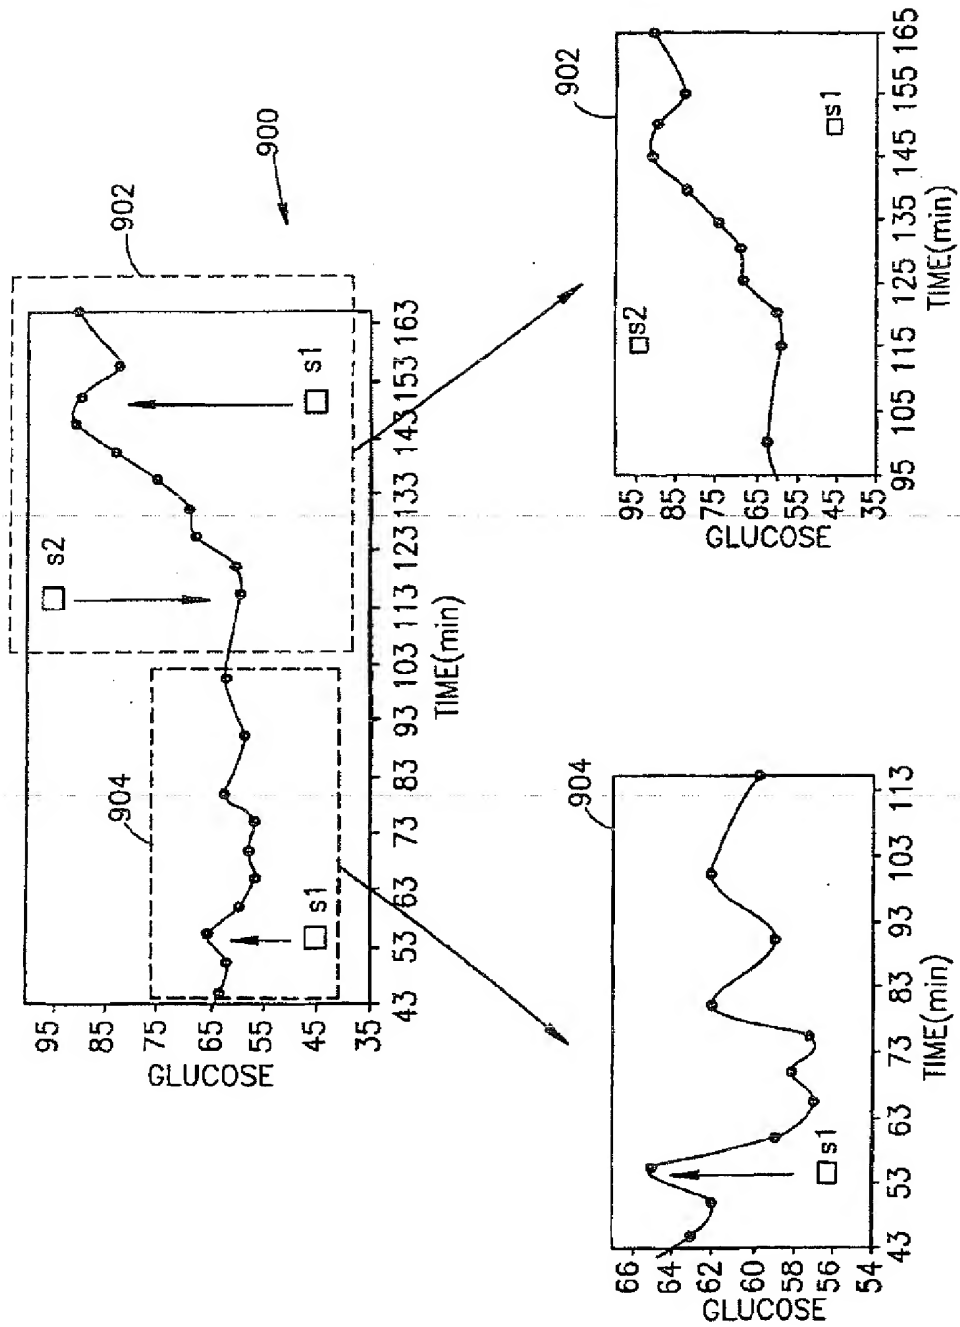


FIG.9

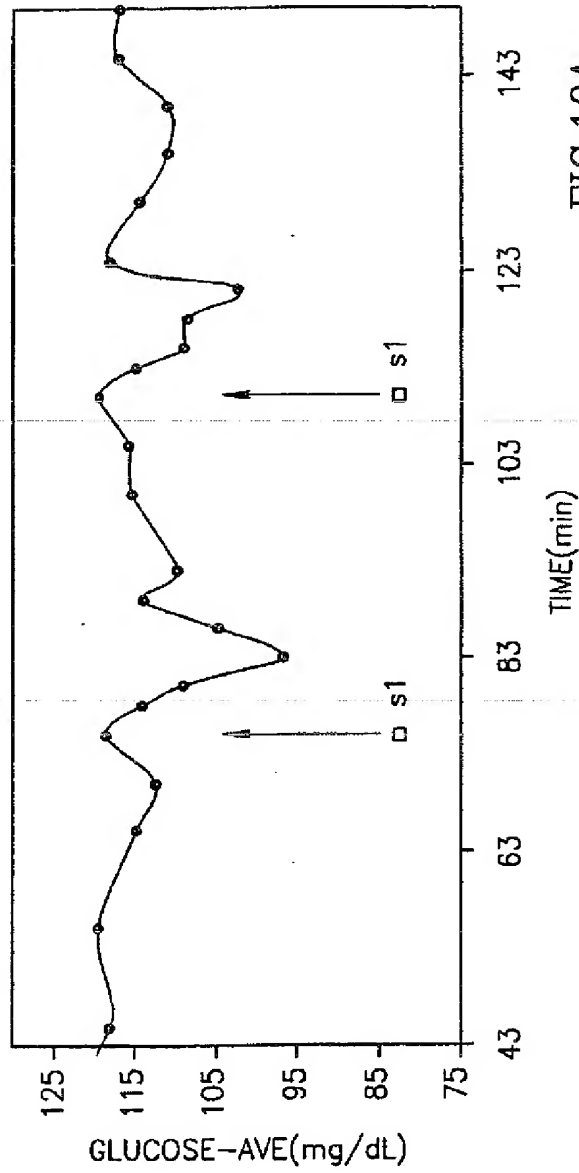


FIG. 10A

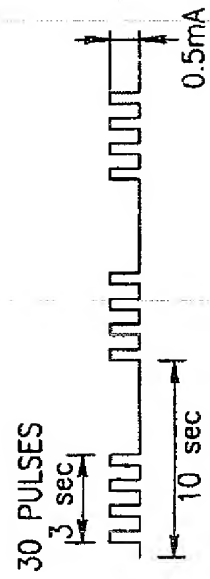


FIG. 10B

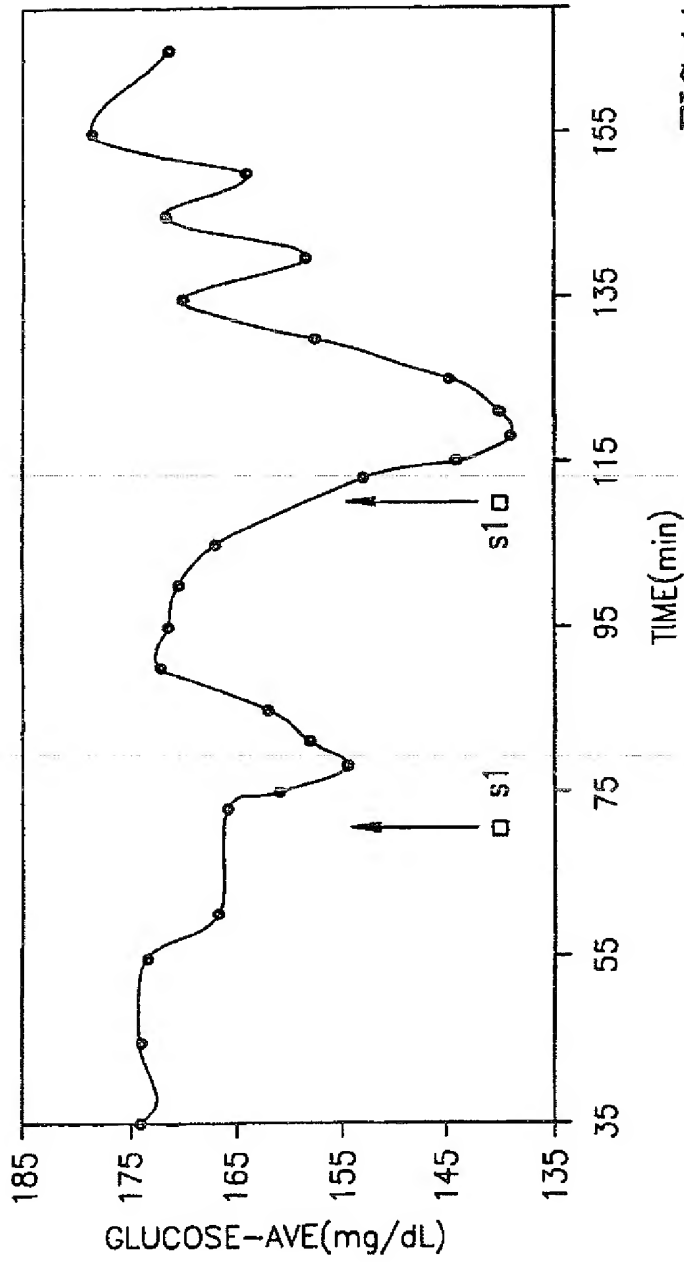


FIG. 11A

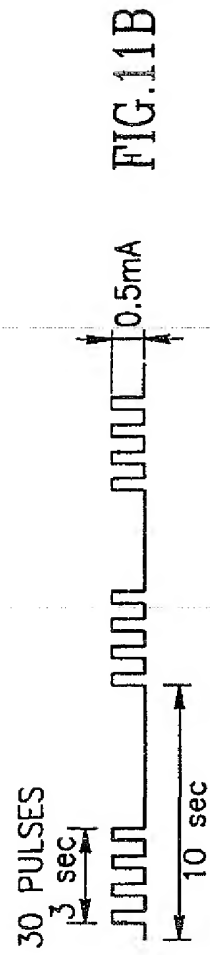
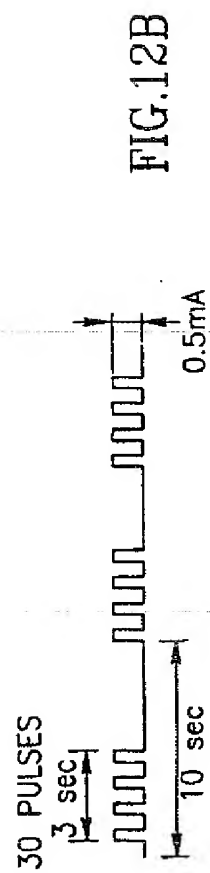
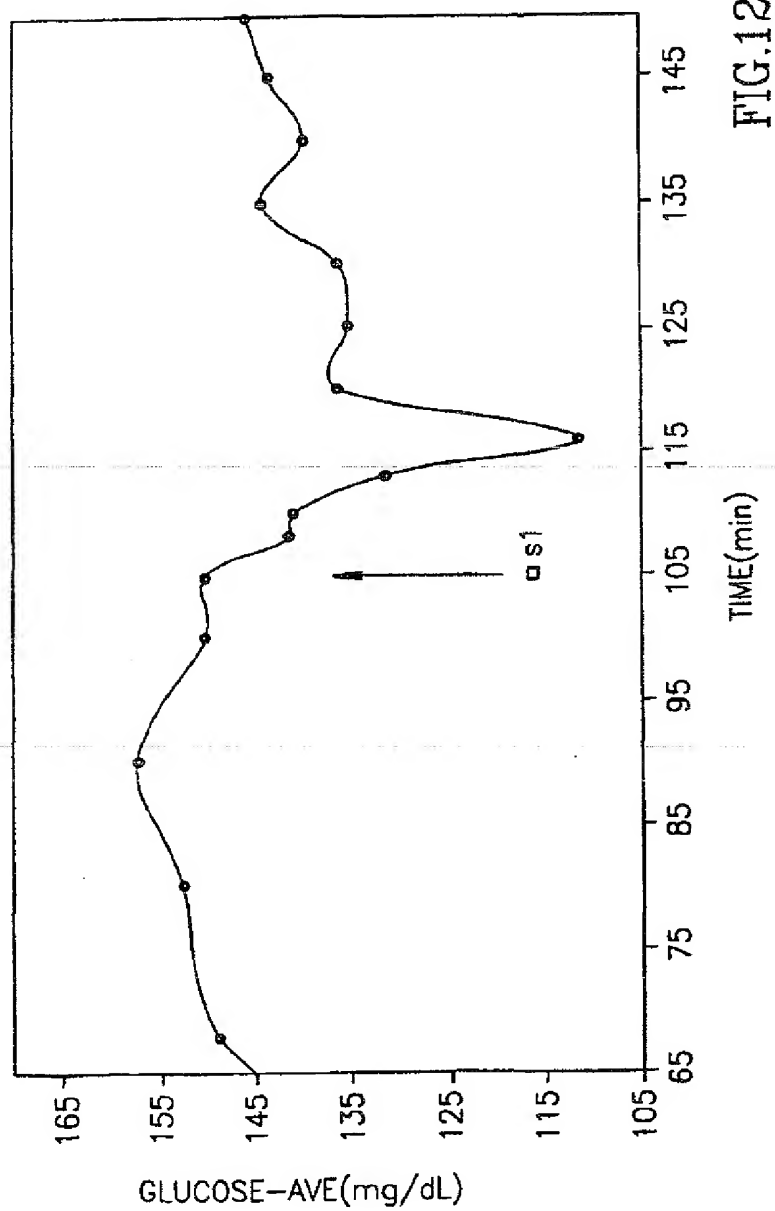


FIG. 11B



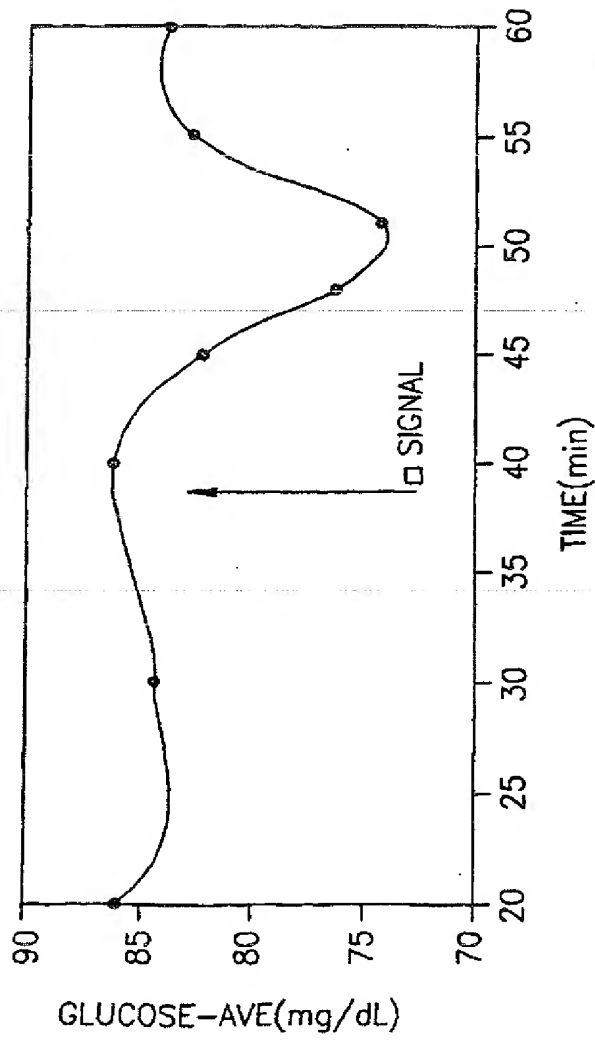


FIG. 13A

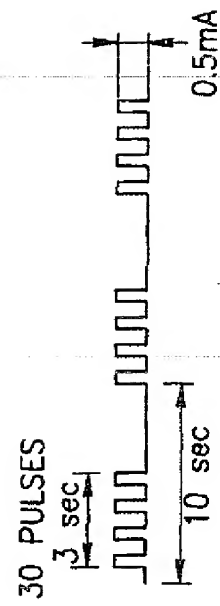


FIG. 13B